

Austin Radiological Association

CT Neuro Protocols

PROTOCOLS

IV Catheter Guidelines	
Carotid/Neck CTA.....	
Cisternogram	
Craniofacial.....	
Dental.....	
Dean Head.....	
Head.....	
Head CTA.....	
Head CTA/ CTV Combo	
Head CTV	
Head and Neck CTA.....	
Head Essential Tremor/Neuravive	
Head Frame Link	
Head Stealth	
Head Synthes Scanning	
Head Trumatch	
Maxillofacial	
Orbits.....	
Sacrum/Coccyx	
Sella.....	
Sinus Complete.....	
Sinus IGS/Medtronic/Stryker.....	
Sinus Limited	
Soft Tissue Neck.....	
4D Neck for Parathyroid Evaluation.....	
Spine Cervical	

- Spine Thoracic.....
- Spine Lumbar.....
- Spine Geck.....
- Spine Mazor.....
- Spine Stealth/Stryker
- Spine Total Combo.....
- Temporal Bones.....
- Temporal Bones Vanderbilt.....
- TMJ.....
- TMJ Concepts.....
- Head DBS Lead.....
- Protocol Review.....

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

IV CATHETER GUIDELINES

Catheter	Injection Rate	PSI
BD Nexiva Diffusics		
24g	Less than or equal to 2cc/sec	325
22g	Less than 4cc/sec	325
20g	Greater than 4cc/sec	325
B Braun Safety Introcan		
24g	HAND INJECTION ONLY	
22g	Less than or equal to 2cc/sec	300
20g	Less than or equal to 4cc/sec	300
18g	Less than or equal to 6cc/sec	300
B Braun Safety 3 Introcan		
24g	Less than or equal to 2.5cc/sec	300
22g	Less than or equal to 3.5cc/sec	300
20g	Less than or equal to 6cc/sec	300

[*Back to Neuro Protocol Page*](#)

CTDI: ~10-25mGy

Setup:

- Neck positioned on flat table top
- Retract shoulders as much as possible
- Head First Supine PA/Lateral scout from below the aortic arch through the bottom half of the orbits

DFOV: Preferred 15 cm (18 cm can be used when the required anatomy is not displayed in a 15cm DFOV)

Exam:

1. CTA Neck

- Scan from the floor of the sella through the level of arch (includes great vessel origins and most of the arch)
- Smart Prep or Bolus Tracking in the descending aorta (trigger set at 80 HU on Siemens) (45 HU on GE)
- 10 second monitoring delay on Bolus Tracking/Smart Prep

Contrast:



- at the discretion of the Radiologist
- 75ml of 320- 370 mg/dl non-ionic contrast @ 5 ml/sec
- See [IV Catheter Guidelines](#)

Injector Setup:

- 30ml Saline Flush @ 5ml/sec
- 75ml Omnipaque 350 @ 5ml/sec
- 100ml Saline Flush @ 5ml/sec

PACS Series:

- 1x1 CTA axial (source Images)
- 1x1 CTA Soft Tissue Coronal MIP
- 1x1 CTA Soft Tissue Sagittal MIP
- 3D Imaging (RT/LT Carotid/Vertebral Slabs, VR Overlay)
- Patient Protocol/Dose Report

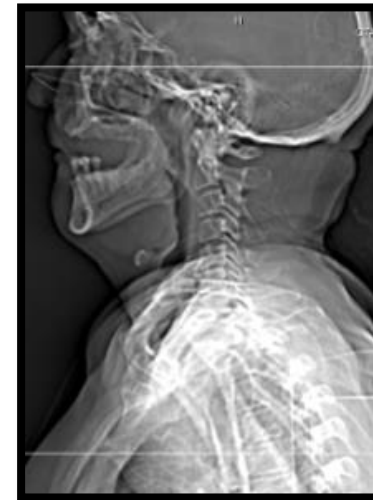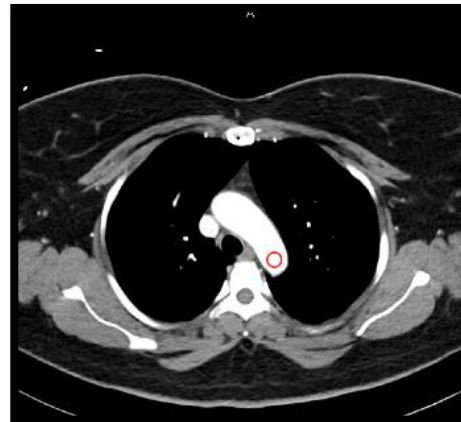

[*Back to Neuro Protocol Page*](#)

CAROTID PROTOCOLS

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	0.5	Rotation Time (sec)	0.5
Pitch	1	1	1	Pitch	0.969:1
Scan FOV	Large	Large	Small	Speed (mm/rot)	19.37
CareDose4D	On	On	On	Scan FOV	Large
Quality ref mAs	150	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	0
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Recon 1 Carotid				Recon 1 ST Carotid	
Kernel	I31f Med Smooth	I31f Med Smooth	I31f Med Smooth	Algorithm	Standard
Window	CT angio	Larynx	Larynx	Window Width/ Level	700/80
SAFIRE/ADMIRE	2	2	2	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Reformat set				Recon 2 Recons	
Kernel	I30f Med Smooth	I30f Med Smooth	I26f Med Smooth	Algorithm	Standard
Window	CT angio	Larynx	Larynx	Window Width/ Level	700/80
SAFIRE/ADMIRE	2	2	1	Slice Thickness (mm)	0.625
Slice Thickness (mm)	0.75	0.75	0.75	Slice Increment (mm)	0.625
Slice Increment (mm)	0.5	0.5	0.5	Type	Plus
Coronal/ Sagittal				ASIR	
Kernel	I31f Med Smooth	I31f Med Smooth	I31f Med Smooth	Recon 3 Bone	
Window	CT angio	angio	CT angio	Algorithm	Bone Plus
SAFIRE/ADMIRE	2	2	2	Window Width/ Level	1500/450
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
				Type	Plus
				ASIR	Full
				Recon 4 ST	
				Algorithm	STND
				Window Width/ Level	700/80
				Slice Thickness (mm)	1.25
				Slice Increment (mm)	0.625
				Type	
				ASIR	Full

CTDI: ~15mGy

****Protocol to be discussed with Performing Radiologist****

****Scan can be done Prone or Supine depending which position they leak****

Setup: 1. Prone, Lateral scout, no gantry angle


2. Scout from tip of the nose through skull

3. Patient Positioning:

- Prone Chin up and/or Supine as requested by the Radiologist ****marker on RT cheek****

4. Scan anterior to the tip of the nose through the ventricles

DFOV: Preferred 25 cm

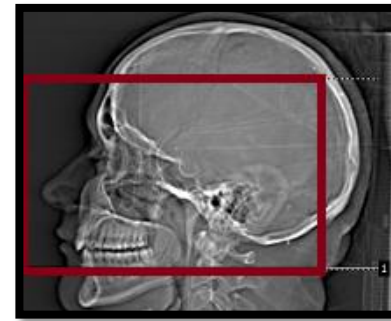

PACS Series

- **1x1 Pre** Coronal Bone, Coronal ST, Axial Bone, Axial ST, Sagittal Bone, Sagittal ST
- **1x1 Post** Coronal Bone, Coronal ST, Axial Bone, Axial ST, Sagittal Bone, Sagittal ST
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

CISTERNOGRAM PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1	1	0.5	Rotation Time (sec)	0.5
Pitch	1	1	1	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	On	On	On	Scan FOV	Large
Quality ref mAs	35	50	125	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		5 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
ST Cor/Sag				Recon 1 ST	
Kernel	I31f Med Smooth	I31f Med Smooth	I31f Med Smooth	Algorithm	Standard
Window	Sinus	Sinus	Sinus	Window Width/ Level	700/80
SAFIRE/ADMIRE	0	0	0	Slice Thickness (mm)	2.5
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	2.5
Slice Increment (mm)	1	1	1	Type	Full
Bone Cor/Sag				ASIR	
Kernel	H70h Very Sharp	H70h Very Sharp	H70h Very Sharp	Recon 2 Bone	
Window	Inner Ear	Inner Ear	Inner Ear	Algorithm	Standard
SAFIRE/ADMIRE	0	0	0	Window Width/ Level	700/80
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
Reformat ST				Type	
Kernel	I31f Med Smooth	I31f Med Smooth	I31f Med Smooth	Full	
Window	Sinus	Sinus	Sinus	ASIR	
SAFIRE/ADMIRE	0	0	0	Recon 3 ST Reformat	
Slice Thickness (mm)	0.75	0.75	0.75	Algorithm	Standard
Slice Increment (mm)	0.5	0.5	0.5	Window Width/ Level	700/80
Reformat Bone				Slice Thickness (mm)	
Kernel	H70h Very Sharp	H70h Very Sharp	H70h Very Sharp	0.625	
Window	Inner Ear	Inner Ear	Inner Ear	Slice Increment (mm)	
SAFIRE/ADMIRE	0	0	0	0.625	
Slice Thickness (mm)	0.75	0.75	0.75	Type	
Slice Increment (mm)	0.5	0.5	0.5	Full	
				ASIR	
				Recon 4 Bone Reformat	
				Algorithm	
				Standard	
				Window Width/ Level	
				700/80	
				Slice Thickness (mm)	
				0.625	
				Slice Increment (mm)	
				0.625	
				Type	
				Full	
				ASIR	

Not to exceed CTDIvol of 15 mGy

This protocol is used when routine Craniofacial, Craniofacial Medical Modeling, BIOMET modeling or Impantech are requested

Setup: PA/Lateral scout from below the mandible through the top of the skull

Place skin marker on the patient's right cheek prior to scanning

Reconstructions:

- 3mm x 3mm Oblique MPR's of the brain should be parallel to the skull base and extend from the skull base through the top of the skull

PACS Series:

- Topogram
- 1x1 Axial Soft Tissue 25cm DFOV (CD Data Set)
- 1x1 Axial Bone
- 1x1 Bone Coronal
- 1x1 Bone Sagittal
- 3x3 Soft Tissue Oblique MPR Axial
- VRT Rotation/Tumble (3D)
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

CRANIOFACIAL PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1	1	1	Rotation Time (sec)	0.5
Pitch	0.85	0.8	0.8	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	On	On	On	Scan FOV	Large
Quality ref mAs	35	35	35	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		130	120	Smart mA	off
Optimize Slider position		5 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				ST Brain	
Kernel	H31s Med Smooth	H31s Med Smooth	J37s Med Smooth	Algorithm	Standard
Window	Sinus	Sinus	Cerebrum	Window Width/ Level	350/40
SAFIRE/ADMIRE	0	0	2	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Bone				ASIR	SS20
Kernel	H70s Med Smooth	J70h Very Sharp	J70h Very Sharp	Bone	
Window	Inner Ear	Inner Ear	Cranial Bone	Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	1	Window Width/ Level	1500/450
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Cor/Sag				Type	Full
Kernel	H70s Med Smooth	J70h Very Sharp	J70h Very Sharp	ASIR	
Window	Inner Ear	Inner Ear	Cranial Bone	3D	
SAFIRE/ADMIRE	0	0	1	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	350/40
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	1.25
Axial Oblique				Slice Increment (mm)	0.6
Kernel	H70s Med Smooth	H31s Med Smooth	J37s Med Smooth	Type	Plus
Window	Cerebrum	Inner Ear	Cerebrum	ASIR	
SAFIRE/ADMIRE	0	0	2	Bone Reformat	
Slice Thickness (mm)	3	3	3	Algorithm	Bone Plus
Slice Increment (mm)	3	3	3	Window Width/ Level	1500/450
Reformat				Slice Thickness (mm)	1.25
Kernel	H70s Med Smooth	H31s Med Smooth	J30s Med Smooth	Slice Increment (mm)	0.6
Window	Cerebrum	Inner Ear	Cerebrum	Type	Plus
SAFIRE/ADMIRE	0	0	1	ASIR	None
Slice Thickness (mm)	0.6	0.6	0.75	ST Reformat	
Slice Increment (mm)	0.3	0.3	0.3	Algorithm	STND

CTDI: ~15 mGy

Setup:

- Supine, lateral scout from below the mandible through the frontal sinuses

Scan parameters:

- Supine helical scan from below the mandible through the frontal sinuses
- 18 cm DFOV is preferred (range 15-22cm)
- If the scan is performed with and without contrast, the bone reconstructions only need to be done on the post-contrast scan

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

****Send Reformat set to SyngoVia****

PACS Series:

- 1x1 Axial Bone
- 1x1 Axial Soft Tissue
- 1x1 Coronal Bone
- 1x1 Sagittal Bone
- Panorex (3d)
- Para- Axial Dental (3d)
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

DENTAL PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1	1	1	Rotation Time (sec)	0.5
Pitch	1	1	1	Pitch	0.969:1
Scan FOV	Large	Large	Small	Speed (mm/rot)	39.37
CareDose4D	On	On	On	Scan FOV	Large
Quality ref mAs	35	50	125	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		5 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial Bone				Dental ST	
Kernel	H70h Very Sharp	H70h Very Sharp	H70h Very Sharp	Algorithm	Standard
Window	Inner Ear	Inner Ear	Inner Ear	Window Width/ Level	350/40
SAFIRE/ADMIRE	0	0	0	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Axial ST				ASIR	
Kernel	I31f Med Smooth	I31f Med Smooth	H41s Med +	Dental Bone	Bone Plus
Window	Sinus	Sinus	Sinuses	Algorithm	1500/450
SAFIRE/ADMIRE	0	0	0	Window Width/ Level	1.25
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	Full
Reformat				Type	SS20
Kernel	I31f Med Smooth	I31f Med Smooth	H70h Very Sharp	ASIR	
Window	Inner Ear	Inner Ear	Inner Ear	Reformat Bone	
SAFIRE/ADMIRE	0	0	0	Algorithm	Standard
Slice Thickness (mm)	0.75	0.75	0.6	Window Width/ Level	1500/450
Slice Increment (mm)	0.3	0.3	0.3	Slice Thickness (mm)	0.625
				Slice Increment (mm)	0.625

CTDI: ~75 mGy

Setup:

- Supine, PA/Lateral scout from below the hard palate thru the head
- Occlusal plane perpendicular to table
- Center at EM
- BB to be placed on the Right Ear

Scan parameters:

- Supine helical scan from below the hard palate to include top of head
- Include tip of nose and back of head
- 25 cm DFOV is preferred / 15 cm DFOV on Unilateral RT/LT


Contrast:

At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 50 second delay



PACS Series:

- Topogram/Scout
- 0.625 x 0.625 Axial Bone through entire head ; 25 DFOV ; WW 350 – WL 50
- 0.5 x 0.5 Coronal Bone through entire head ; 25 DFOV ; WW 350 – WL 50
- 0.5 x 0.5 Sagittal Bone through entire head ; 25 DFOV ; WW 350 – WL 50
- 0.5 x 0.5 Right Coronal Oblique Temporal Bone ; 15 DFOV ; WW 4000 – WL 700
- 0.5 x 0.5 Left Coronal Oblique Temporal Bone ; 15 DFOV ; WW 4000 – WL 700
- 0.5 x 0.5 Right Sagittal Oblique Temporal Bone ; 15 DFOV ; WW 4000 – WL 700
- 0.5 x 0.5 Left Sagittal Oblique Temporal Bone ; 15 DFOV ; WW 4000 – WL 700
- Dose report
- ***PT to take CD- 1st CD with Axial Data only, 2nd CD with everything***

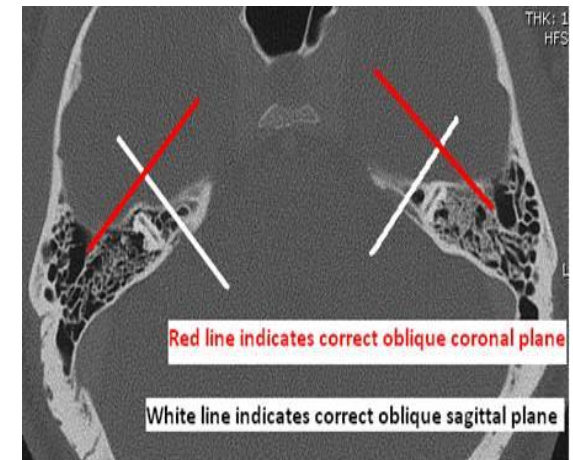

****SEE ATTACHED PROTOCOL BELOW FOR SCAN SPECIFIC REQUIREMENTS**

[*Back to Neuro Protocol Page*](#)

CT Dean Protocol

Positioning

Occlusal plane perpendicular to table
Center at EM

Scan Region

Include top of the head to the hard palate
Include tip of nose and back of the head

Raw Scan Data

Axial, Helical Scan

Thickness 0.625
Interval: 0.625
Speed: 10.62 @ 0.531:1
SFOV: Head
kV: 140 WW: 350 WL: 50

mA: 400auto
Total Exposure Time: 5.64
Noise Index: 7.00
Smart mA: Turn On
CTDI Volume: 75

Recon 2 (Thins)

Thickness: 0.625
Interval: 0.312
Recon Type: Bone Plus

Recon option: Full IQ Enhance Plus
WW: 4000 WL: 700

Reformats

Coronal – through entire head (tip of nose to back of head) 0.5 X 0.5 – 25FOV – 4000W 700L
Sagittal – through entire head (top of head to the hard palate) 0.5 X 0.5 – 25 FOV – 4000W 700L
Stenver – R and L sides – 0.5 X 0.5 – 15 FOV – 4000W 700L
Poschl – R and L sides – 0.5 X 0.5 – 15 FOV – 4000W 700L

 **When finished with this exam please burn one CD with the Raw Axial Sequence and One CD with everything.** 

[*Back to Neuro Protocol Page*](#)

CTDI: ~35-60mGy (do not exceed the ACR recommended 75mGy)

Setup:

1. Supine, PA/Lateral scouts
2. Patient Positioning: Tilt the patients head so that a line connecting the lateral canthus of the eye and the EAC is perpendicular to the CT tabletop (see below). Angle the gantry if you cannot place the patient's head within 15 degrees of the proper setup angle.
3. Start scans at the bottom of the skull base and scan through the top of the head


DFOV: Preferred 20 cm (Range 18-22)

Contrast:

1. at the discretion of the Radiologist
2. 100 ml of 350 mg iodine/ml non-ionic contrast
3. Minimum 5 minute delay after the administration of IV contrast
4. See [IV Catheter Guidelines](#)



Coronals-line dorsum sellae to
Anterior arch of C1 line or perpendicular to hard palate

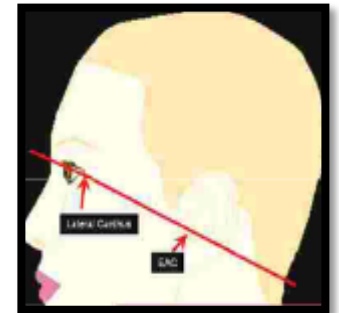

Positioning

PACS Series:

- 3x3 Brain
- 3x3 Bone (Only needed on one series not both)
- 3X3 Coronal ST
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

HEAD PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
				Recon 1 Brain	
Axial Brain				Algorithm	Standard
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Window Width/ Level	80/35
Window	Cerebrum	Cerebrum	Cerebrum	Slice Thickness (mm)	2.5
SAFIRE/ADMIRE	0	0	2	Slice Increment (mm)	2.5
Slice Thickness (mm)	3	3	3	Type	Full
Slice Increment (mm)	3	3	3	ASIR	SS30
				Recon 2 Bone	
Axial Bone				Algorithm	Bone
Kernel	J80s Very Sharp	J70h Very Sharp	J70h Very Sharp	Window Width/ Level	3000/800
Window	Cranial bone	Cranial bone	Cranial bone	Slice Thickness (mm)	2.5
SAFIRE/ADMIRE	0	0	1	Slice Increment (mm)	2.5
Slice Thickness (mm)	3	3	3	Type	Full
Slice Increment (mm)	3	3	3	ASIR	SS20
				Recon 2 Trauma Reformat	
Coronal ST				Algorithm	STND
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Window Width/ Level	100/50
Window	Cerebrum	Cerebrum	Cerebrum	Slice Thickness (mm)	1.25
SAFIRE/ADMIRE	0	0	2	Slice Increment (mm)	0.625
Slice Thickness (mm)	3	3	3	Type	Full
Slice Increment (mm)	3	3	3	ASIR	None

CTDI: ~ 30-50 mGy / acquisition

Setup

- Head First Supine
- See [CT Head Protocol](#) for scan and reconstruction parameters

DFOV: Preferred 20 cm

Exam:


- Routine Brain without contrast
- CTA Head Only
 - Scan from C1 through the top of the head (NO GANTRY TILT)
 - Smart Prep or Bolus Tracking in descending aorta at the aortic arch (trigger set to 60 HU on Siemens) (50 HU on GE)
 - 10 second monitoring delay on Bolus Tracking/Smart Prep
- Routine Post Contrast Brain @ 5 minutes

Contrast:

- at the discretion of the Radiologist
 - 50ml Omnipaque 350 @ 5ml/sec [*See IV Catheter Guidelines*](#)
 - 100ml Saline Flush @ 5ml/sec

PACS Series:


- Topogram
- 3x3 Pre contrast brain
- 1x1 CTA Axial source images
- 1x1 CTA Coronal/Sagittal MIP
- 16 x1 CTA Axial Oblique MIP
- 3x3 Post contrast brain
- 3x3 Bone (Only needed on the post contrast brain)
- Dose Report




Scan Range



1x1 Coronal MIP



1x1 Sagittal MIP



16x1 CTA Axial Oblique

[*Back to Neuro Protocol Page*](#)

HEAD CTA PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	0.5	Rotation Time (sec)	0.5
Pitch	0.8	0.3	1	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	19.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	275	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial/Cor/Sag					
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	Recon 1 Brain	
Window	cerebrum	cerebrum	Base Orbita	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	1	3	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	3	1	Slice Increment (mm)	2.5
Axial Oblique				Type	Full
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	ASIR	SS30
Window	cerebrum	Cerebrum	Base Orbita		
SAFIRE/ADMIRE	2	0	2	Recon 2 Angio	
Slice Thickness (mm)	16	16	16	Algorithm	Standard
Slice Increment (mm)	1	1	1	Window Width/ Level	450/60
Reformat				Slice Thickness (mm)	1.25
Kernel	J30s	J37sMedsmooth	H20f Smooth	Slice Increment (mm)	1.25
Window	cerebrum	Cerebrum	Cerebrum	Type	Full
SAFIRE/ADMIRE	2	0	0	ASIR	None
Slice Thickness (mm)	3	3	0.75		
Slice Increment (mm)	3	3	0.5	Recon CTA Brain	
Pre/Post Contrast Brain				Algorithm	Standard
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	Window Width/ Level	700/80
Window	cerebrum	Cerebrum	Cerebrum	Slice Thickness (mm)	0.625
SAFIRE/ADMIRE	2	0	2	Slice Increment (mm)	0.625
Slice Thickness (mm)	3	3	3	Type	Plus
Slice Increment (mm)	3	3	3	ASIR	SS30
Post Contrast Bone					
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp		
Window	Cranial bone	Cranial bone	Cranial Bone		
SAFIRE/ADMIRE	2	0	1		
Slice Thickness (mm)	1	3	3		
Slice Increment (mm)	1	3	3		


Setup:

- Head First Supine
- See [CT Head Protocol](#) for scan and reconstruction parameters

DFOV: Preferred 20 cm

Exam:

- Routine Brain without contrast
- CTA Head Only (NO TILT)
 - Scan from **C1** through the top of the head
 - Smart Prep or Bolus Tracking in descending aorta at the aortic arch (trigger set to 60 HU on Siemens) (50 HU on GE)
 - 10 second monitoring delay on Bolus Tracking/Smart Prep
- CTV Head (NO TILT)
 - Scan from C1 through the top of the head immediately following completion of CTA
- Routine Post Contrast Brain @ 5 minutes



Scan Range


Contrast:

- at the discretion of the Radiologist
- 75 ml of 350 mg iodine/ml non-ionic contrast @ 5 ml/sec [*See IV Catheter Guidelines](#)




Injector Setup:


- 30 ml Saline Flush @ 5ml/sec
- 75 ml Omnipaque 350 @ 5ml/sec
- 100 ml Saline Flush @ 5ml/sec



1x1 Coronal MIP



1x1 Sagittal MIP



16x1 Axial Oblique MIP

PACS Series:

- Topogram
- 3x3 Pre contrast brain
- 1x1 CTA Axial source images
- 1x1 CTA Coronal MIP
- 1x1 CTA Sagittal MIP
- 16x1 CTA Axial Oblique MIP
- 1x1 CTV Axial source images
- 1x1 CTV Coronal MIP
- 1x1 CTV Sagittal MIP
- 3x3 Post contrast brain
- 3x3 Bone (Only needed on the post contrast brain)
- 3D lab will create and submit CPR, VRT and MIP images
- Dose Report

[*Back to Neuro Protocol Page*](#)

HEAD CTA/CTV PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	19.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	275	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CTA/CTV Axial/Cor/Sag					
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	Recon 1 Brain	
Window	Cerebrum	Cerebrum	Base Orbita	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	1	3	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	3	1	Slice Increment (mm)	2.5
Axial Oblique					
Kernel	J30s	J37sMedsmooth	J37f Med Smooth	Type	Full
Window	Cerebrum	Cerebrum	Base Orbita	ASIR	SS30
SAFIRE/ADMIRE	2	0	2	Angio Brain	
Slice Thickness (mm)	16	16	16	Algorithm	Standard
Slice Increment (mm)	1	1	1	Window Width/ Level	450/60
Reformat					
Kernel	J30s	J37sMedsmooth	H20f Smooth	Slice Thickness (mm)	1.25
Window	Cerebrum	Cerebrum	Cerebrum	Slice Increment (mm)	1.25
SAFIRE/ADMIRE	2	0	0	Type	Full
Slice Thickness (mm)	3	3	0.75	ASIR	None
Slice Increment (mm)	3	3	0.5	Venogram Brain	
Pre/Post Contrast Brain					
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Cerebrum	Window Width/ Level	450/60
SAFIRE/ADMIRE	2	0	2	Slice Thickness (mm)	1.25
Slice Thickness (mm)	3	3	3	Slice Increment (mm)	1.25
Slice Increment (mm)	3	3	3	Type	Full
Post Contrast Bone					
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp	ASIR	None
Window	Cranial bone	Cranial bone	Cranial Bone	Reformat	
SAFIRE/ADMIRE	2	0	1	Algorithm	Standard
Slice Thickness (mm)	3	3	3	Window Width/ Level	700/80
Slice Increment (mm)	3	3	3	Slice Thickness (mm)	0.625
				Slice Increment (mm)	0.625

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~55mGy / acquisition


Setup:

- Head First Supine
- See [CT Head Protocol](#) for scan and reconstruction parameters

DFOV: Preferred 20 cm

Exam:

- Routine Brain without contrast
- CTV Head (NO GANTRY TILT)
 - Scan from C1 through the top of the head
- Routine Post Contrast Brain
 - 5 minute delay

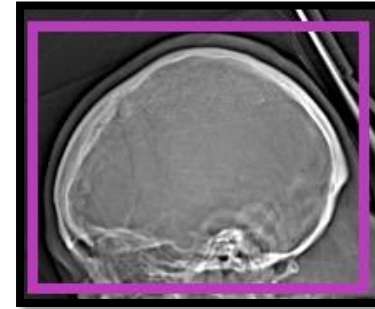

Contrast:

- *At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast@4ml/sec with a 45 second scan delay
- See [IV Catheter Guidelines](#)

PACS Series:

- Topogram
- 3x3 Pre contrast brain
- 1x1 CTV Axial source images
- 1x1 CTV Coronal MIP
- 1x1 CTV Sagittal MIP
- 3x3 Post contrast brain
- 3x3 Bone (Only needed on the post contrast scan)
- Protocol Page/Dose Report

[*Back to Neuro Protocol Page*](#)

HEAD VENOGRAM PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	19.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	275	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CTV Axial/Cor/Sag					
Kernel	J30s	J37s Medsmooth	J37f Med Smooth	Recon 1 Brain	
Window	cerebrum	cerebrum	Base Orbita	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	1	3	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	3	1	Slice Increment (mm)	2.5
Axial Oblique				Type	Full
Kernel	J30s	J37s Medsmooth	J37s Med Smooth	ASIR	SS30
Window	cerebrum	Cerebrum	Base Orbita	CTV Brain	
SAFIRE/ADMIRE	2	0	2	Algorithm	Standard
Slice Thickness (mm)	3	3	3	Window Width/ Level	700/80
Slice Increment (mm)	3	3	1	Slice Thickness (mm)	1.25
Reformat				Slice Increment (mm)	1.25
Kernel	J30s	J37s Medsmooth	J30f Med Smooth	Type	Full
Window	cerebrum	Cerebrum	Base Orbita	ASIR	None
SAFIRE/ADMIRE	2	0	2	Reformat	
Slice Thickness (mm)	3	3	0.75	Algorithm	Standard
Slice Increment (mm)	3	3	0.5	Window Width/ Level	700/80
Pre/Post Contrast Brain				Slice Thickness (mm)	0.625
Kernel	J30s	J37s Medsmooth	J37s Med Smooth	Slice Increment (mm)	0.625
Window	cerebrum	Cerebrum	Cerebrum	Type	Plus
SAFIRE/ADMIRE	2	0	2	ASIR	SS30
Slice Thickness (mm)	3	3	3		
Slice Increment (mm)	3	3	3		
Post Contrast Bone					
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp		
Window	Cranial bone	Cranial bone	Cranial Bone		
SAFIRE/ADMIRE	2	0	1		
Slice Thickness (mm)	3	3	3		
Slice Increment (mm)	3	3	3		

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~ 20-50 mGy / acquisition

Setup:

- Head first Supine
- See [CT Head Protocol](#) for Routine head scan and reconstruction parameters

DFOV: Preferred 20 cm (Range 18-22)

Exam:


1. Routine Brain without contrast
2. CTA Head and Neck
 - Scan from the top of the head through the level of the arch (includes great vessel origins and most of the arch)
 - Smart Prep or Bolus Tracking in the Descending aorta (trigger set at 40 HU on Siemens) (40 HU on GE)
 - 10 second monitoring delay on Bolus Tracking/Smart Prep
 - Routine Post Contrast Brain @ a 5 minute delay

Contrast:

- at the discretion of the Radiologist
- 100ml of 350 mg iodine/ml non-ionic contrast @ 5ml/sec *See [IV Catheter Guidelines](#)
- 30ml Saline Flush @ 5ml/sec
- 100ml Omnipaque 350 @ 5ml/sec
- 100ml Saline Flush @ 5ml/sec

PACS Series:

- Topogram
- 3x3 Pre contrast (Brain)
- 1x1 CTA axial (source images)
- 1x1 Coronal MIP
- 1x1 Sagittal MIP
- 16 x 1 Axial Oblique MIP (Brain)
- 3x3 Post contrast (Brain) / 3x3 Post Contrast Bone (Head only)
- Patient Protocol/Dose Report

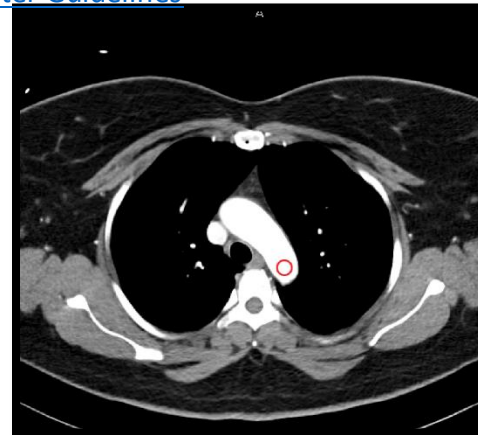

[*Back to Neuro Protocol Page*](#)

HEAD AND NECK CTA PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	275	Auto mA range	100/400
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	19
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CTA Axial/Cor/Sag					
Kernel	J30s	J37sMedsmooth	I31f Med Smooth	Brain S	
Window	cerebrum	cerebrum	Larynx	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	1	3	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	3	1	Slice Increment (mm)	2.5
Axial Oblique					
Kernel	J30s	J37sMedsmooth	I31f Med Smooth	Type	Full
Window	cerebrum	Cerebrum	CT Angio	ASIR	SS30
SAFIRE/ADMIRE	2	0	2	Angio Brain/Carotids	
Slice Thickness (mm)	16	16	16	Algorithm	Standard
Slice Increment (mm)	1	1	1	Window Width/ Level	700/80
Reformat					
Kernel	J30s	J37sMedsmooth	J26f Med Smooth	Slice Thickness (mm)	1.25
Window	cerebrum	Cerebrum	Larynx	Slice Increment (mm)	1.25
SAFIRE/ADMIRE	2	0	2	Type	Plus
Slice Thickness (mm)	3	3	0.75	ASIR	SS10
Slice Increment (mm)	3	3	0.5	Reformat Brain	
Pre/Post Contrast Brain					
Kernel	J30s	J37sMedsmooth	J37s Med Smooth	Algorithm	Standard
Window	cerebrum	Cerebrum	Cerebrum	Window Width/ Level	700/80
SAFIRE/ADMIRE	2	0	2	Slice Thickness (mm)	0.625
Slice Thickness (mm)	3	3	3	Slice Increment (mm)	0.625
Slice Increment (mm)	3	3	3	Type	Plus
Post Contrast Bone					
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp	ASIR	SS30
Window	Cranial bone	Cranial bone	Cranial Bone	Reformat Carotid	
SAFIRE/ADMIRE	2	0	1	Algorithm	Standard
Slice Thickness (mm)	3	3	3	Window Width/ Level	700/80
Slice Increment (mm)	3	3	3	Slice Thickness (mm)	0.625
				Slice Increment (mm)	0.625

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

MRgFUS, Essential Tremor, HIFU, Neuravive, for SDR or similar. *

CTDI: ~60mGy (do not exceed the ACR recommended 75mGy)

a) Contrast: No Contrast

b) Acquisition Direction: helical or axial mode.

c) Inter-slice resolution: 1mm continuous (Thickness=1mm, Spacing=1mm, No overlap, no gaps). A smaller slice size reformatted into a 1 mm set is allowed.

I. For GE: 0.625mm thickness is preferred. If 0.625 mm is unavailable, 1.25 mm is acceptable

d) Kernel / Filter: Post-processed using only the following specific 'Bone' filters:

I. For 'GE' CT machine – use only 'BonePlus' filter

II. For 'Siemens' CT machine – use only 'H60' or 'H60s' i. with a newer model- use 'Hr59' or Hr60 filter

III. For 'Philips' CT machine – use only 'C or C-Sharp' or 'UC' filter

IV. For 'Toshiba/Canon' CT machine – use only 'FC30' filter

e) Alignment: Roughly aligned on supine patient along orbitomeatal line

f) Matrix Size: symmetrical matrix no larger than 512 x 512

g) Coverage: Axial range from air slices above superior most scalp down to skull base, inclusive

I. GE Revolution only – Ensure FOV is set to 'head'

Tilt: No preference for Gantry tilt – a rough alignment as above will suffice on most patients

Providing data to the patient a) Only Axial dataset in the correct kernel & reformatted in 1mm slices needed. A typical set is 150-200 slices b) Decompressed datasets preferred. c) DICOM reader and additional datasets are not needed, but may be included as per normal site protocols d) Two identical disks should be provided to the patient. Verification of these parameters will occur after the treating site receives the disk from the patient. This may take a few weeks. If possible, please DO NOT DELETE ORIGINAL / RAW DATA from the modality until the image set has been verified, such as to allow for reprocessing if necessary

[*Back to Neuro Protocol Page*](#)

HEAD ESSENTIAL TREMOR/NEURAVIVE PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				CD Data Set	
Kernel	J37s Med Smooth	J37s Med Smooth	H60s Sharp FR	Algorithm	Bone Plus
Window	Cerebrum	Cerebrum	Cranial Bone	Window Width/ Level	3000/800
SAFIRE/ADMIRE	0	0	0	Slice Thickness (mm)	2.5
Slice Thickness (mm)	3	3	1	Slice Increment (mm)	2.5
Slice Increment (mm)	3	3	1	Type	Full
Axial Brain ST				ASIR	None
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	ST	
Window	Cerebrum	Cerebrum	Cerebrum	Algorithm	Standard
SAFIRE/ADMIRE	0	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	3	3	3	Slice Thickness (mm)	2.5
Slice Increment (mm)	3	3	3	Slice Increment (mm)	2.5
				Type	Full
				ASIR	SS30
				Recon 2 Trauma Reformat	
				Algorithm	STND
				Window Width/ Level	100/50
				Slice Thickness (mm)	1.25
				Slice Increment (mm)	0.625
				Type	Full
				ASIR	None

CTDI: ~45 mGy

Setup:

- Head first supine, PA/Lateral scout from below the skull base through the top of the skull,
 - **Only use the flat sponge, No Gantry Tilt**

Scan Parameters:

- Begin Below skull base and extend through the top of the skull

DFOV:


- 25-32 cm DFOV is used for the CD Data set. Include the entire nose and ears
- 20 cm DFOV is used for all other series

Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- Topogram
- CD Data Set
 - 1x1 (1.25 x 1.25) Axial Soft Tissue 25-32cm DFOV
- 3 x 3 Axial ST 20cm DFOV
- 3 x 3 Axial ST 20cm DFOV
- Patient Protocol/Dose Report

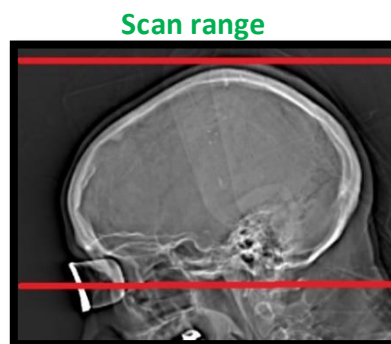

[*Back to Neuro Protocol Page*](#)

HEAD FRAME LINK PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				Recon 1 Brain	
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Cerebrum	Window Width/ Level	80/35
SAFIRE/ADMIRE	0	0	2	Slice Thickness (mm)	2.5
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	2.5
Slice Increment (mm)	1	1	1	Type	Full
Axial Brain				ASIR	SS30
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Recon 2 Bone	
Window	Cerebrum	Cerebrum	Cerebrum	Algorithm	Bone
SAFIRE/ADMIRE	0	0	2	Window Width/ Level	3000/800
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
Bone Axial/Cor/Sag				Type	Full
Kernel	J80s Very Sharp	J70h Very Sharp	J70h Very Sharp	ASIR	SS20
Window	Cranial Bone	Cranial Bone	Cranial Bone	Recon 2 Trauma Reformat	
SAFIRE/ADMIRE	0	0	1	Algorithm	STND
Slice Thickness (mm)	1	1	1	Window Width/ Level	100/50
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	1.25
				Slice Increment (mm)	0.625
				Type	Full
				ASIR	None

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~10-20 mGy


Place skin marker on the patient's right cheek prior to scanning

Setup:

- Head first supine , lateral scout from below the chin through the top of the skull
- Patient positioned so that the IOML is perpendicular to the table top
 - Only use the flat sponge

Scan Parameters:

- Scan range should begin below the chin and extend through the top of the skull
- DFOV
 - 25-30 cm DFOV is used for the CD Data set. Include the entire nose and ears
 - 15-17 cm DFOV is used for all other series

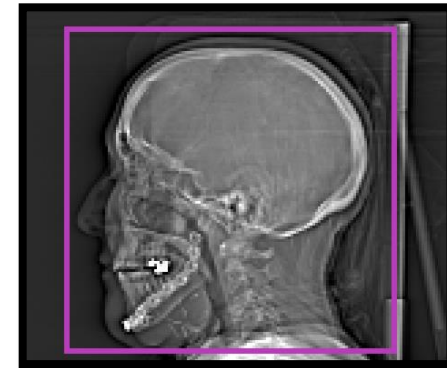

Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- Topogram
- CD Data Set
 - 1x1 Axial Soft Tissue 25cm DFOV
- 0.5 x0.5 Axial Bone 17cm DFOV
- 1 x 1 Coronal Bone 15cm DFOV
- 1 x 1 Sagittal Bone 15cm DFOV
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

HEAD STEALTH PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				CD Data Set	
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Cerebrum	Window Width/ Level	80/40
SAFIRE/ADMIRE	0	0	2	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Axial Brain				ASIR	SS10
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Axial Bone	
Window	Cerebrum	Cerebrum	Cerebrum	Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	2	Window Width/ Level	1500/450
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Bone Axial/Cor/Sag				Type	Plus
Kernel	J80s Very Sharp	J70h Very Sharp	J70h Very Sharp	ASIR	None
Window	Cranial Bone	Cranial Bone	Cranial Bone	Bone Reformat	
SAFIRE/ADMIRE	0	0	1	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	1500/450
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	1.25
				Slice Increment (mm)	0.6
				Type	Plus
				ASIR	None

CTDI: ~55 mGy (do not exceed ACR recommended 75mGy)

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Head first supine , PA/Lateral scout from below the chin through the top of the skull
- Tilt the patients head so that a line connecting the lateral canthus of the eye and the EAC are perpendicular to the CT tabletop

Scan Parameters:

- Scan range should begin below the area of interest and extend through the top of the head

DFOV:

- To include the entire skull

PACS Series:

- Topogram
- CD Data Set
- ST Brain
- Bone
- Patient Protocol/Dose Report

HEAD SYNTHES PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				Recon 1 Brain	
Kernel	J37s Med Smooth	J37s Med Smooth	H70h Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Cranial Bone	Window Width/ Level	80/35
SAFIRE/ADMIRE	0	0	0	Slice Thickness (mm)	2.5
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	2.5
Slice Increment (mm)	0.5	0.5	0.5	Type	Full
Axial Brain				ASIR	SS10
Kernel	J37s Med Smooth	J37s Med Smooth	J37s Med Smooth	Recon 2 Bone	
Window	Cerebrum	Cerebrum	Cerebrum	Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	2	Window Width/ Level	1500/450
Slice Thickness (mm)	3	3	3	Slice Thickness (mm)	2.5
Slice Increment (mm)	3	3	3	Slice Increment (mm)	2.5
Bone Axial/Cor/Sag				Type	Full
Kernel	J80s Very Sharp	J70h Very Sharp	J70h Very Sharp	ASIR	None
Window	Cranial bone	Cranial bone	Cranial Bone	CD Data Set	
SAFIRE/ADMIRE	0	0	1	Algorithm	Bone Plus
Slice Thickness (mm)	3	3	3	Window Width/ Level	1500/450
Slice Increment (mm)	3	3	3	Slice Thickness (mm)	1.25
				Slice Increment (mm)	1.25
				Type	Full
				ASIR	None

CTDI: ~10-20 mGy


Place skin marker on the patient's right cheek prior to scanning

Setup:

- Head first supine, PA/Lateral scout from below the chin through the top of the skull
- Patient positioned so that the IOML is perpendicular to the table top
 - Only use the flat sponge, no straps

Scan Parameters:

- Scan range should begin below the chin and extend through the top of the skull
- NO GANTRY TILT
- Rotation of 1
- DFOV
 - 25 cm DFOV is used for the CD Data set.
 - 15-17 cm DFOV is used for all other series

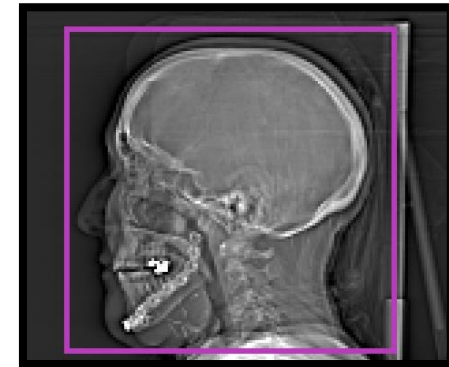

Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- Topogram
- 1x1 Axial Bone CD Data Set 25cm DFOV (1.25x1.25 for GE)
- 1x1 Axial ST (1.25x1.25 for GE)
- 1x1 Coronal/Sagittal Bone (1.25x1.25 for GE)
- 1x1 Coronal/Sagittal ST (1.25x1.25 for GE)
- 3D Tumble/Rotation
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

HEAD TRUMATCH PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	19.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	275	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set				CD Data Set	
Kernel	J30s	J37s Medsmooth	J70h Very Sharp	Algorithm	Bone Plus
Window	cerebrum	cerebrum	Osteo	Window Width/ Level	4000/700
SAFIRE/ADMIRE	2	2	2	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Axial ST				ASIR	SS20
Kernel	J30s	J37s Medsmooth	J37s Med Smooth	ST Reformat	
Window	cerebrum	Cerebrum	Cerebrum	Algorithm	Standard
SAFIRE/ADMIRE	2	2	2	Window Width/ Level	280/35
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	0.625
Slice Increment (mm)	1	1	1	Slice Increment (mm)	0.625
Cor/Sag Bone				Type	Full
Kernel	J30s	J37s Medsmooth	J70h Very Sharp	ASIR	SS20
Window	cerebrum	Cerebrum	Cranial Bone	Bone Reformat	
SAFIRE/ADMIRE	1	1	1	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	4000/700
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	1.25
Cor/Sag ST				Slice Increment (mm)	0.625
Kernel	J30s	J37s Medsmooth	J37s Med Smooth	Type	Plus
Window	cerebrum	Cerebrum	Cerebrum	ASIR	None
SAFIRE/ADMIRE	2	2	2	3D Reformat	
Slice Thickness (mm)	1	1	1	Algorithm	Standard
Slice Increment (mm)	1	1	1	Window Width/ Level	280/35
Reformat				Slice Thickness (mm)	0.625
Kernel	J80s verysharp	J70h verysharp	J30s Med Smooth	Slice Increment (mm)	0.625
Window	Cranial bone	Cranial bone	Cerebrum		
SAFIRE/ADMIRE	2	2	2		
Slice Thickness (mm)	0.75	0.75	0.75		
Slice Increment (mm)	0.3	0.3	0.3		

CTDI: ~15 mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Supine, PA/Lateral scout from below the mandible through the frontal sinuses

Scan parameters:

- Supine helical scan from below the mandible through the frontal sinuses
- 18 cm DFOV is preferred
- If the scan is performed with and without contrast, the bone reconstructions only need to be done on the post-contrast scan

Contrast:

At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- 1x1 Axial Bone
- 1x1 Axial Soft Tissue
- 1x1 Coronal Bone
- 1x1 Coronal Soft Tissue
- 1x1 Sagittal Bone
- 1x1 Sagittal Soft Tissue
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

MAXILLOFACIAL PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.8	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
ST Axial				Recon Axial ST	
Kernel	J37s Med Smooth	J37s Med Smooth	H31s Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Sinuses	Window Width/ Level	350/40
SAFIRE/ADMIRE	0	0	0	Slice Thickness (mm)	1.25
Slice Thickness (mm)	1	1	1	Slice Increment (mm)	1.25
Slice Increment (mm)	1	1	1	Type	Full
Bone Axial				ASIR	None
Kernel	J80s Very Sharp	J70h Very Sharp	H70h Very Sharp	Recon Bone	
Window	Cranial bone	Cranial bone	Inner Ear	Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	0	Window Width/ Level	1500/450
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
ST Cor/Sag				Type	Full
Kernel	J37s Med Smooth	J37s Med Smooth	H31s Med Smooth	ASIR	None
Window	Cerebrum	Cerebrum	Sinuses	Recon Reformat Bone	
SAFIRE/ADMIRE	0	0	0	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	1500/450
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	0.625
Bone Cor/Sag				Slice Increment (mm)	0.625
Kernel	J80s Very Sharp	J70h Very Sharp	H70h Very Sharp	Type	Full
Window	Cranial bone	Cranial bone	Inner Ear	ASIR	None
SAFIRE/ADMIRE	0	0	0	Recon Reformat ST	
Slice Thickness (mm)	1	1	1	Algorithm	STND
Slice Increment (mm)	1	1	1	Window Width/ Level	350/40
				Slice Thickness (mm)	0.625

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~15 mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Supine, PA/Lateral scout from below the mandible through the frontal sinuses

Scan parameters:


- Supine helical scan from below the maxillary sinuses through the frontal sinuses
- 18 cm DFOV is preferred
- If the scan is performed with and without contrast, the bone reconstructions only need to be done on the post-contrast scan

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- 1x1 Axial Bone
- 1x1 Axial Soft Tissue
- 1x1 Coronal Bone
- 1x1 Coronal Soft Tissue
- 1x1 Sagittal Bone
- 1x1 Sagittal Soft Tissue
- Patient Protocol/Dose Report

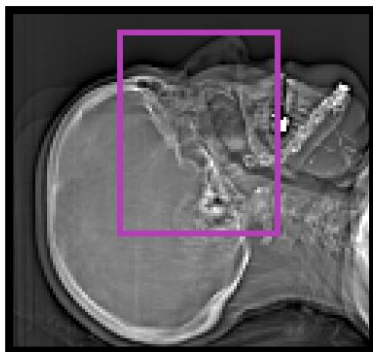

[*Back to Neuro Protocol Page*](#)

ORBIT PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1		Rotation Time (sec)	0.5
Pitch	0.55	1	0.8		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	off	off	off		Scan FOV	Large
Quality ref mAs	190	225	275		Auto mA range	100-500
kVp	130				kVp	120
ref kVp		120	120		Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
ST Axial					Recon Axial ST	
Kernel	J37s Med Smooth	J37s Med Smooth	H31s Med Smooth		Algorithm	Standard
Window	Cerebrum	Cerebrum	Sinuses		Window Width/ Level	280/35
SAFIRE/ADMIRE	0	0	0		Slice Thickness (mm)	2.5
Slice Thickness (mm)	1	1	1		Slice Increment (mm)	2.5
Slice Increment (mm)	1	1	1		Type	Full
Bone Axial					ASIR	SS20
Kernel	J80s Very Sharp	J70h Very Sharp	H70h Very Sharp		Axial Bone	
Window	Cranial bone	Cranial bone	Inner Ear		Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	0		Window Width/ Level	1500/450
Slice Thickness (mm)	1	1	1		Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1		Slice Increment (mm)	2.5
ST Cor/Sag					Type	Full
Kernel	J37s Med Smooth	J37s Med Smooth	H31s Med Smooth		ASIR	None
Window	Cerebrum	Cerebrum	Sinuses		Recon Reformat Bone	
SAFIRE/ADMIRE	0	0	0		Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1		Window Width/ Level	1500/450
Slice Increment (mm)	1	1	1		Slice Thickness (mm)	0.625
Bone Cor/Sag					Slice Increment (mm)	0.625
Kernel	J80s Very Sharp	J70h Very Sharp	H70h Very Sharp		Type	Full
Window	Cranial bone	Cranial bone	Inner Ear		ASIR	None
SAFIRE/ADMIRE	0	0	0		Recon Reformat ST	
Slice Thickness (mm)	1	1	1		Algorithm	STND
Slice Increment (mm)	1	1	1		Window Width/ Level	280/35
					Slice Thickness (mm)	0.625

CTDI: ~15-30 mGy

Setup:

- Scout from below the coccyx through L1 with the patients arms raised above their head

Scan Parameters:

- Scan from below the coccyx to L4
- DFOV should include SI joints
- For patients with implanted spinal hardware and/or a BMI ≥ 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help maintain image quality <http://www.nhlbisupport.com/bmi/bminojs.htm>

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Axial Sacrum Soft Tissue
- 2x2 Axial Sacrum Bone
- 2X2 Sagittal Sacrum
- 2x2 Coronal Sacrum
- Patient Protocol/Dose Report

Axial Soft Tissue




Axial Bone



Sagittal Sacrum



Coronal Sacrum

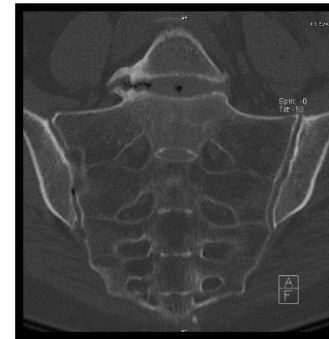

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

SACRUM/COCCYX PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	on	on	on		Scan FOV	Large
Quality ref mAs	190	125	125		Auto mA range	100-500
kVp	110				kVp	120
ref kVp		120	120		Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
Axial ST						
Kernel	J30s	J37sMedsmooth	I41s Medium		Recon 1 Sacrum/Coccyx	
Window	cerebrum	cerebrum	Spine		Algorithm	Standard
SAFIRE/ADMIRE	0	0	0		Window Width/ Level	350/40
Slice Thickness (mm)	2	2	2		Slice Thickness (mm)	2.5
Slice Increment (mm)	2	2	2		Slice Increment (mm)	2.5
Axial Bone					Type	Full
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp		ASIR	SS10
Window	Cranial bone	Cranial bone	Osteo			
SAFIRE/ADMIRE	2	2	0		Recon Bone	
Slice Thickness (mm)	2	2	2		Algorithm	Bone Plus
Slice Increment (mm)	2	2	2		Window Width/ Level	1500/450
Reformat					Slice Thickness (mm)	2.5
Kernel	J30s	J37sMedsmooth	B50s Med Sharp		Slice Increment (mm)	2.5
Window	cerebrum	Cerebrum	Osteo		Type	Full
SAFIRE/ADMIRE	2	2	0		ASIR	None
Slice Thickness (mm)	0.75	0.75	0.6			
Slice Increment (mm)	0.5	0.5	0.6		Reformat	
Cor/Sag					Algorithm	Detail
Kernel	J80s verysharp	J70h verysharp	I50s Med Sharp		Window Width/ Level	1500/450
Window	Cranial bone	Cranial bone	Osteo		Slice Thickness (mm)	1.25
SAFIRE/ADMIRE	2	2	0		Slice Increment (mm)	0.625
Slice Thickness (mm)	2	2	2		Type	Plus
Slice Increment (mm)	2	2	2		ASIR	None

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*



SELLA/PITUITARY – Revised-5/16/2024

CTDI: ~45mGy

Not to exceed the ACR recommended dose of 75 mGy

Setup:

- Supine, PA/Lateral scout from below the maxillary sinuses through the frontal sinuses

Scan parameters:

- Supine helical scan from below the maxillary sinuses through the frontal sinuses
- 15 cm DFOV is preferred
- If the scan is performed with and without contrast, the bone reconstructions only need to be done on the post-contrast scan, axial, coronal and sagittal soft tissue on **both** pre and post contrast

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350-370 mg iodine/ml non-ionic contrast @ 4 ml/sec with a **25 second delay**
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Axial Soft Tissue
- 2x2 Axial Bone
- 2x2 Soft tissue Coronal
- 2x2 Soft Tissue Sagittal
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

SELLA/PITUITARY PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	225	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
ST Axial				Axial ST	
Kernel	J37s Med Smooth	J37s Med Smooth	J30s Med Smooth	Algorithm	Standard
Window	Cerebrum	Cerebrum	Cerebrum	Window Width/ Level	280/35
SAFIRE/ADMIRE	2	2	2	Slice Thickness (mm)	2.5
Slice Thickness (mm)	2	2	2	Slice Increment (mm)	2.5
Slice Increment (mm)	2	2	2	Type	Full
Bone Axial				ASIR	SS10
Kernel	J80s Very Sharp	J70h Very Sharp	H70h Very Sharp	Recon Bone	
Window	Cranial bone	Cranial bone	Cranial Bone	Algorithm	Bone Plus
SAFIRE/ADMIRE	0	0	0	Window Width/ Level	1500/450
Slice Thickness (mm)	2	2	2	Slice Thickness (mm)	2.5
Slice Increment (mm)	2	2	2	Slice Increment (mm)	2.5
ST Cor/Sag				Type	Full
Kernel	J37s Med Smooth	J37s Med Smooth	J30s Med Smooth	ASIR	None
Window	Cerebrum	Cerebrum	Cerebrum	Recon Reformat Bone	
SAFIRE/ADMIRE	2	2	2	Algorithm	Bone Plus
Slice Thickness (mm)	2	2	2	Window Width/ Level	1500/450
Slice Increment (mm)	2	2	2	Slice Thickness (mm)	0.625
				Slice Increment (mm)	0.625
				Type	Full
				ASIR	None
				Recon Reformat ST	
				Algorithm	STND
				Window Width/ Level	280/35
				Slice Thickness (mm)	1.25

CTDI: ~15- 20 mGy


Place skin marker on the patient's right cheek prior to scanning

Setup:

- Supine, Lateral/PA Scout, No gantry angle
- Scout from below mandible through the frontal sinuses
- Supine helical scan to include entire paranasal sinuses parallel to the hard palate, inclusive of the upper teeth

Scan Parameters:

- 15cm DFOV Preferred
- Supine helical scan from below upper teeth through frontal sinus
- Only perform the bone reconstructions on the post contrast scan if the exam is performed without and with IV contrast

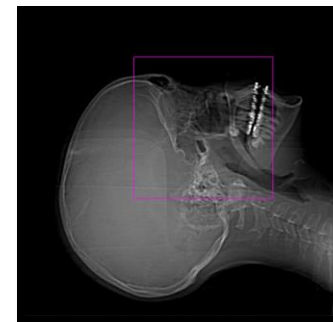


Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

**For Sagittal Reconstruction the radiologists request to be parallel to hard palate- see image

PACS Series:

- Scout/Topogram
- 1x1 Axial Bone
- 1x1 Axial ST
- 1x1 Coronal Bone
- 1x1 Coronal ST
- 1x1 Sagittal Bone
- 1x1 Sagittal ST
- Patient Protocol/Dose Report

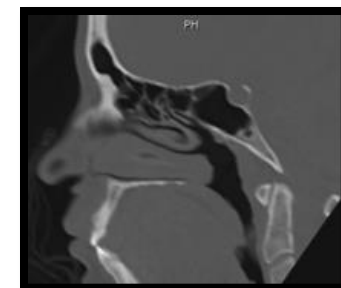

[*Back to Neuro Protocol Page*](#)

SINUS COMPLETE PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660	
Scan Type	spiral	spiral	spiral		Scan Type	spiral	
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20	
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5	
Pitch	0.8	0.3	0.8		Pitch	0.969:1	
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37	
CareDose4D	on	on	on		Scan FOV	Large	
Quality ref mAs	190	125	125		Auto mA range	100-500	
kVp	110				kVp	120	
ref kVp		120	120		Smart mA	off	
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18	
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%	
Axial ST					Coronal Sinus		
Kernel	J30s	J37s Medsmooth	H31s Medsmooth		Algorithm	Bone Plus	
Window	cerebrum	cerebrum	Sinuses		Window Width/ Level	4000/700	
SAFIRE/ADMIRE	2	0	0		Slice Thickness (mm)	1.25	
Slice Thickness (mm)	1	1	1		Slice Increment (mm)	0.625	
Slice Increment (mm)	1	1	1		Type	Full	
Axial Bone					ASIR	SS10	
Kernel	J80s verysharp	J70h verysharp	H70h Very Sharp		Coronal ST		
Window	Cranial bone	Cranial bone	Inner Ear		Algorithm	Standard	
SAFIRE/ADMIRE	2	0	0		Window Width/ Level	280/35	
Slice Thickness (mm)	1	1	1		Slice Thickness (mm)	1.25	
Slice Increment (mm)	1	1	1		Slice Increment (mm)	0.625	
Cor/Sag ST					Type	Plus	
Kernel	J30s	J37s Medsmooth	H31s Medsmooth		ASIR	SS20	
Window	cerebrum	cerebrum	Sinuses		Cor/Sag Bone		
SAFIRE/ADMIRE	2	0	0		Kernel	J80s verysharp	
Slice Thickness (mm)	1	1	1		Window	Cranial bone	
Slice Increment (mm)	1	1	1		SAFIRE/ADMIRE	2	
Cor/Sag Bone					Slice Thickness (mm)	1	
Kernel	J80s verysharp	J70h verysharp	H70h Very Sharp		Slice Increment (mm)	1	
Window	Cranial bone	Cranial bone	Inner Ear				
SAFIRE/ADMIRE	2	0	0				
Slice Thickness (mm)	1	1	1				
Slice Increment (mm)	1	1	1				

CTDI: ~10-20 mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Head first supine , lateral scout from below the mandible through the top of the skull,
 - [Only use the flat sponge](#)

Scan Parameters:

- For **IGS Sinuses the Scan range** should begin below the teeth and extend through the entire frontal sinuses
- For **Medtronic and Stryker Sinuses Scan range** should begin below the teeth and extend through the top of the skull
- DFOV
 - 25-30 cm DFOV is used for the CD Data set. Include the entire nose and ears
 - 15 cm DFOV is used for all other series

Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

No piercings allowed due to surgical computer/robot limitations in reading images if metal is present

PACS Series:

Topogram

- CD Data Set
 - 1x1 Axial Soft Tissue 25cm DFOV
- 1 x 1 Axial Bone 15cm DFOV
- 1 x 1 Coronal Bone 15cm DFOV
- 1 x 1 Sagittal Bone 15cm DFOV
- 1 x 1 Axial ST 15cm DFOV
- 1 x 1 Coronal ST 15cm DFOV
- 1 x 1 Sagittal ST 15cm DFOV
- Patient Protocol/Dose Report


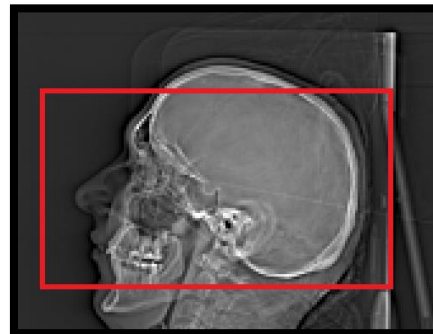


Image Guided Sinus/IGS Scan Range

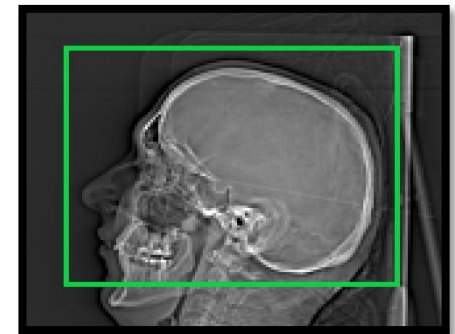

Medtronic/Stryker Scan range

[*Back to Neuro Protocol Page*](#)

SINUS IMAGE GUIDED/MEDTRONIC/STRYKER PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set					
Kernel	J30s	J37sMedsmooth	H31s Medsmooth	Sinus IGS Data Set	
Window	cerebrum	cerebrum	Sinuses	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	280/35
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	H70h Very Sharp	ASIR	SS20
Window	Cranial bone	Cranial bone	Inner Ear	ST Reformat	
SAFIRE/ADMIRE	2	0	0	Algorithm	Standard
Slice Thickness (mm)	1	1	1	Window Width/ Level	280/35
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	0.625
Cor/Sag ST				Slice Increment (mm)	0.625
Kernel	J30s	J37sMedsmooth	H31s Medsmooth	Type	Plus
Window	cerebrum	cerebrum	Sinuses	ASIR	SS20
SAFIRE/ADMIRE	2	0	0	Bone Reformat	
Slice Thickness (mm)	1	1	1	Algorithm	Bone Plus
Slice Increment (mm)	1	1	1	Window Width/ Level	4000/700
Cor/Sag Bone				Slice Thickness (mm)	0.625
Kernel	J80s verysharp	J70h verysharp	H70h Very Sharp	Slice Increment (mm)	0.625
Window	Cranial bone	Cranial bone	Inner Ear	Type	Plus
SAFIRE/ADMIRE	2	0	0	ASIR	None
Slice Thickness (mm)	1	1	1		
Slice Increment (mm)	1	1	1		

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~5-15mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Head first prone, lateral scout to include the entire nose and extend beyond the EAM

Scan Parameters:


- Scan starts anterior to the tip of the nose and extends through the adenoids
- 15 cm DFOV is Preferred

Contrast:

- At the discretion of the radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series:

- Scout/Topogram
- 3x3Coronal Bone
- 3x3Coronal ST
- Patient Protocol/Dose Report

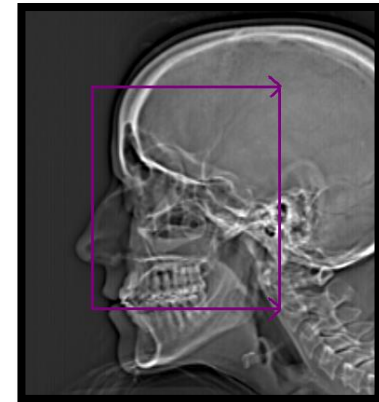

[*Back to Neuro Protocol Page*](#)

SINUS LIMITED PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	on	on	on		Scan FOV	Large
Quality ref mAs	190	125	125		Auto mA range	100-500
kVp	110	100	100		kVp	120
ref kVp		120	120		Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
Coronal ST						
Kernel	J30s	J37sMedsmooth	H31s Medsmooth		Coronal Sinus	
Window	cerebrum	cerebrum	Sinuses		Algorithm	Bone Plus
SAFIRE/ADMIRE	2	0	0		Window Width/ Level	4000/700
Slice Thickness (mm)	3	3	3		Slice Thickness (mm)	1.25
Slice Increment (mm)	3	3	3		Slice Increment (mm)	0.625
Coronal Bone					Type	Full
Kernel	J80s verysharp	J70h verysharp	H70h Very Sharp		ASIR	SS10
Window	Cranial bone	Cranial bone	Inner Ear			
SAFIRE/ADMIRE	2	0	0		Coronal ST	
Slice Thickness (mm)	3	3	3		Algorithm	Standard
Slice Increment (mm)	3	3	3		Window Width/ Level	280/35
					Slice Thickness (mm)	1.25
					Slice Increment (mm)	0.625
					Type	Plus
					ASIR	SS10

CTDI: ~5-25 mGy

Setup:

- *Place skin marker on any mass or region of interest*
- Supine, PA/Lateral scout from above the orbital roof to below the aortic arch

Patient Positioning:

- Retract shoulders as much as possible and tilt the patient's head so that a line connecting the lateral canthus of the eye and the EAC is perpendicular to the CT tabletop

DFOV: Preferred 22 cm (Range 17-24 cm)

Scan Parameters:

1. Non-Contrast scan will be performed at the discretion of the radiologist
2. Perform post contrast acquisition from above the orbital roof to below the aortic arch **with the patient instructed not to swallow**
3. **A dental tilt** scan should be acquired if the patient presents with obstructive dentition

Contrast:

- at the discretion of the Radiologist
 - Injection volume of 50-150 ml of 350 mg iodine/ml non-ionic contrast @ a rate of 2ml/sec, not to exceed a total volume of 150cc for a single exam
 - Scan delay 90 seconds after the start of contrast
- 4.

PT weight in LBS	Volume of contrast
1-50	1 cc/lb
51-100	50cc
101-210	75cc
211-300	100cc
301-400	125cc
>401	150cc

PACS Series:

1. 3x3 (2.5 x 2.5) Axial Soft Tissue
2. 3x3 (2.5 x 2.5) Axial Bone
3. 3x3 (2.5 x 2.5) Coronal Soft Tissue
4. 3x3 (2.5 x 2.5) Sagittal Soft Tissue
5. 2x2 (2.5 x 2.5) Axial Oblique Vocal Cord
 - **If the patient presents with a diagnosis or indication of hoarseness, vocal cord paralysis, or dysphonia an additional axial reconstruction will be performed. The Axial Oblique Vocal Cord reconstruction should be parallel to the cervical spine disc space and extend from the hyoid through the bottom of the cricoid**
6. 3x3 (2.5 x 2.5) Dental Tilt
7. Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

SOFT TISSUE NECK PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	0.5		Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.5		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	on	on	on		Scan FOV	Large
Quality ref mAs	190	125	125		Auto mA range	100-500
kVp	110				kVp	120
ref kVp		120	120		Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
Axial ST						
Kernel	J30s	J37sMedsmooth	I41f Medium		Axial ST	
Window	cerebrum	cerebrum	Larynx		Algorithm	Standard
SAFIRE/ADMIRE	2	0	0		Window Width/ Level	350/40
Slice Thickness (mm)	3	3	3		Slice Thickness (mm)	2.5
Slice Increment (mm)	3	3	3		Slice Increment (mm)	2.5
Axial Bone					Type	Full
Kernel	J80s verysharp	J70h verysharp	I70f Very Sharp AS		ASIR	SS20
Window	Cranial bone	Cranial bone	Cranial Bone			
SAFIRE/ADMIRE	2	0	0		Bone	
Slice Thickness (mm)	3	3	3		Algorithm	Bone Plus
Slice Increment (mm)	3	3	3		Window Width/ Level	1500/450
Cor/Sag ST					Slice Thickness (mm)	2.5
Kernel	J30s	J37sMedsmooth	I41f Medium		Slice Increment (mm)	2.5
Window	cerebrum	cerebrum	Larynx		Type	Full
SAFIRE/ADMIRE	2	0	0		ASIR	None
Slice Thickness (mm)	3	3	3			
Slice Increment (mm)	3	3	3		Reformat	
Dental					Algorithm	Standard
Kernel	J80s verysharp	J70h verysharp	I41f Medium		Window Width/ Level	350/40
Window	Cranial bone	Cranial bone	Larynx		Slice Thickness (mm)	1.25
SAFIRE/ADMIRE	2	0	0		Slice Increment (mm)	0.625
Slice Thickness (mm)	3	3	3		Type	Plus
Slice Increment (mm)	3	3	3		ASIR	SS20

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

Setup:

- Before scheduling, patient must have had a Parathyroid scan and US, if images done @ non ARA facility, priors must be obtained and reviewed by a radiologist
- If no prior exams, radiologist approval is needed to proceed and must be documented in tech notes

DFOV: Preferred 20cm (Range 19-21cm)

Scan Parameters: Images to be obtained from carina through the bottom of the mandibular teeth while patient breathes normally

- Non-contrast
- 25 Second Scan (after start of injection)
- 50 Second Scan (after start of injection)
- 80 Second Scan (after start of injection)
- 110 Second Scan (after start of injection)

Contrast:

- At the discretion of the Radiologist inject 120 ml of omnipaque 350 mg iodine/ml non-ionic contrast @ 4 ml/sec
- See [IV Catheter Guidelines](#)

PACS Series:

- Non-Contrast Axial, Coronal & Sagittal 1x1
- 25 Second Axial, Coronal & Sagittal 1x1
- 50 Second Axial, Coronal & Sagittal 1x1
- 80 Second Axial, Coronal & Sagittal 1x1
- 110 Second Axial, Coronal & Sagittal 1x1
- Patient Protocol/Dose Report

4D NECK PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	0.5	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial ST					
Kernel	J30s	J37sMedsmooth	I41f Medium	Axial	
Window	cerebrum	cerebrum	Larynx	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	350/40
Slice Thickness (mm)	1	3	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	3	1	Slice Increment (mm)	1.25
Coronal					
Kernel	J80s verysharp	J70h verysharp	I31f Med Smooth	Type	Full
Window	Cranial bone	Cranial bone	Larynx	ASIR	SS20
SAFIRE/ADMIRE	2	0	0	Reformat	
Slice Thickness (mm)	1	3	1	Algorithm	Standard
Slice Increment (mm)	1	3	1	Window Width/ Level	350/40
Sagittal					
Kernel	J30s	J37sMedsmooth	I41f Medium	Slice Thickness (mm)	1.25
Window	cerebrum	Cerebrum	Larynx	Slice Increment (mm)	0.625
SAFIRE/ADMIRE	2	0	0	Type	Plus
Slice Thickness (mm)	3	3	1	ASIR	SS20
Slice Increment (mm)	3	3	1		

Setup:

- Do not flex or extend the neck if there has been recent spine trauma or if the patient is in a cervical collar
- Retract shoulders as much as possible
- Scout from T3 through the skull base

Scan Parameters:

- Scan from just below T1 Through the entire cervical spine
- Preferred DFOV is 12 cm

Contrast: At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second scan delay

- See [IV Catheter Guidelines](#)


Reformats:

- Oblique Axial images should be reformatted when the spine is not in plane during the initial acquisition. Images below are an example of the correct plane for reformatting oblique axial images when the spine is not in the true axial plane during acquisition

PACS Series:

- 1x1 Axial Cervical Soft Tissue
- 1x1 Axial Cervical Bone
- 1x1 Coronal/Sagittal
- 1x1 RT/LT Obliques
- 1x1 Oblique Axial(s) As needed
- Patient Protocol/Dose Report

****For all spines with hardware-please send Reformat set to Terarecon****

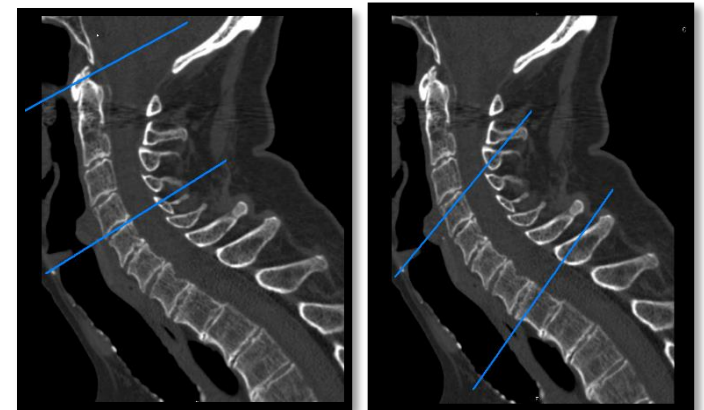

[*Back to Neuro Protocol Page*](#)

SPINE - CERVICAL PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.65	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial ST					
Kernel	J30s	J37sMedsmooth	I41s Medium	Cervical	
Window	cerebrum	cerebrum	Spine	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	350/40
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	ASIR	SS10
Window	Cranial bone	Cranial bone	Osteo		
SAFIRE/ADMIRE	2	0	0	Bone	
Slice Thickness (mm)	1	1	1	Algorithm	Bone Plus
Slice Increment (mm)	1	1	1	Window Width/ Level	1500/450
Reformat				Slice Thickness (mm)	1.25
Kernel	J30s	J37sMedsmooth	B50s Med Sharp	Slice Increment (mm)	1.25
Window	cerebrum	Cerebrum	Osteo	Type	Full
SAFIRE/ADMIRE	2	0	0	ASIR	None
Slice Thickness (mm)	0.75	0.75	0.75		
Slice Increment (mm)	0.5	0.5	0.5	Reformat	
Cor/Sag/Obl				Algorithm	Detail
Kernel	J30s	J37sMedsmooth	I50s Med Sharp	Window Width/ Level	1500/450
Window	cerebrum	Cerebrum	Osteo	Slice Thickness (mm)	0.625
SAFIRE/ADMIRE	2	0	1	Slice Increment (mm)	0.625
Slice Thickness (mm)	1	1	1	Type	Plus
Slice Increment (mm)	1	1	1	ASIR	None

CTDI: ~15-30 mGy

Setup:

- Post Myelography patients must be rolled 360 degrees to help evenly distribute spinal contrast
- Scout from S2 through the mid cervical spine with the patient's arms raised above their head

Scan Parameters:

- Scan from L1 to C6
- Preferred DFOV of 17 cm
- For patients with implanted spinal hardware and/or a BMI ≥ 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help to maintain image quality <http://www.nhlbisupport.com/bmi/bminojs.htm>

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Axial Thoracic Soft Tissue
- 2x2 Axial Thoracic Bone
- 2X2 Sagittal Thoracic Spine
- 2x2 Coronal Thoracic Spine
- Patient Protocol/Dose Report

****For all spines with hardware-please send Reformat set to Terarecon****



[*Back to Neuro Protocol Page*](#)

SPINE - THORACIC PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial ST				Axial ST	
Kernel	J30s	J37sMedsmooth	I41s Medium	Algorithm	Standard
Window	cerebrum	cerebrum	Spine	Window Width/ Level	350/40
SAFIRE/ADMIRE	2	0	0	Slice Thickness (mm)	2.5
Slice Thickness (mm)	2	2	2	Slice Increment (mm)	2.5
Slice Increment (mm)	2	2	2	Type	Full
Axial Bone				ASIR	SS10
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	Bone	
Window	Cranial bone	Cranial bone	Osteo	Algorithm	Bone Plus
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	1500/450
Slice Thickness (mm)	2	2	2	Slice Thickness (mm)	2.5
Slice Increment (mm)	2	2	2	Slice Increment (mm)	2.5
Reformat				Type	Full
Kernel	J30s	J37sMedsmooth	B50s Med Sharp	ASIR	None
Window	cerebrum	Cerebrum	Osteo	Reformat	
SAFIRE/ADMIRE	2	0	0	Algorithm	Detail
Slice Thickness (mm)	1	1	1	Window Width/ Level	1500/450
Slice Increment (mm)	0.7	0.7	0.7	Slice Thickness (mm)	1.25
Cor/Sag				Slice Increment (mm)	0.625
Kernel	J30s	J37sMedsmooth	I50s Med Sharp	Type	Plus
Window	cerebrum	Cerebrum	Osteo	ASIR	None
SAFIRE/ADMIRE	2	0	0		
Slice Thickness (mm)	2	2	2		
Slice Increment (mm)	2	2	2		

CTDI: ~15-30 mGy

Setup:

- Post Myelography patients must be rolled 360 degrees to help evenly distribute spinal contrast
- Scout from S2 through T8 with the patients arms raised above their head

Scan Parameters:


- Scan from S2 through the mid body of T12
- Preferred DFOV of 17 cm
- For patients with implanted spinal hardware and/or a BMI ≥ 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help maintain image quality <http://www.nhlbisupport.com/bmi/bminojs.htm>

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Axial Lumbar Soft Tissue
- 2x2 Axial Lumbar Bone
- 2X2 Sagittal Lumbar Spine
- 2x2 Coronal Lumbar Spine
- 2x2 Axial Oblique 1
- Patient Protocol/Dose Report

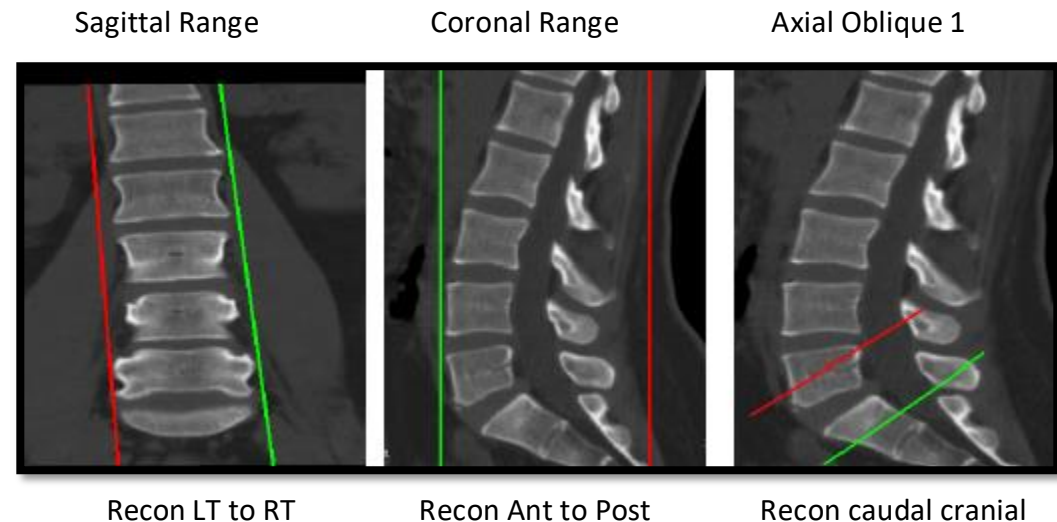

****For all spines with hardware-please send Reformat set to Terarecon****

[*Back to Neuro Protocol Page*](#)

SPINE - LUMBAR PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	on	on	on		Scan FOV	Large
Quality ref mAs	190	125	125		Auto mA range	100-500
kVp	110				kVp	120
ref kVp		120	120		Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
Axial ST						
Kernel	J30s	J37sMedsmooth	I41s Medium		Axial ST	
Window	cerebrum	cerebrum	Spine		Algorithm	Standard
SAFIRE/ADMIRE	2	0	0		Window Width/ Level	350/40
Slice Thickness (mm)	2	2	2		Slice Thickness (mm)	2.5
Slice Increment (mm)	2	2	2		Slice Increment (mm)	2.5
Axial Bone					Type	Full
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp		ASIR	SS10
Window	Cranial bone	Cranial bone	Osteo			
SAFIRE/ADMIRE	2	0	0		Bone	
Slice Thickness (mm)	2	2	2		Algorithm	Bone Plus
Slice Increment (mm)	2	2	2		Window Width/ Level	1500/450
Reformat					Slice Thickness (mm)	2.5
Kernel	J30s	J37sMedsmooth	B50s Med Sharp		Slice Increment (mm)	2.5
Window	cerebrum	Cerebrum	Osteo		Type	Full
SAFIRE/ADMIRE	2	0	0		ASIR	None
Slice Thickness (mm)	1	1	1			
Slice Increment (mm)	0.7	0.7	0.7		Reformat	
Cor/Sag/Obl					Algorithm	Detail
Kernel	J30s	J37sMedsmooth	I50s Med Sharp		Window Width/ Level	1500/450
Window	cerebrum	Cerebrum	Osteo		Slice Thickness (mm)	1.25
SAFIRE/ADMIRE	2	0	0		Slice Increment (mm)	0.625
Slice Thickness (mm)	2	2	2		Type	Plus
Slice Increment (mm)	2	2	2		ASIR	None

CTDI: ~15-30 mGy

Setup:

- Post Myelography patients must be rolled 360 degrees to help evenly distribute spinal contrast
- Scout with the patients arms raised above their head or down by side for cervical only

Scan Parameters:


- Preferred DFOV of 17 cm
- For Adults use MAS greater than 400
- ****For lumbar axial oblique imaging of the lower three screws should be scanned and NOT reformatted** see image below**
- For patients with implanted spinal hardware and/or a BMI ≥ 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help maintain image quality <http://www.nhlbisupport.com/bmi/bminojs.htm>

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Lumbar/Thoracic or 1x1 Cervical Axial ST
- 2x2 Lumbar/Thoracic or 1x1 Cervical Axial Bone
- 2x2 Lumbar/Thoracic or 1x1 Cervical Coronal Spine
- 2x2 Lumbar/Thoracic or 1x1 Cervical Sagittal Spine
- 1x1 Cervical RT/LT Oblique
- Curved Coronal/Sagittal
- 3D Hardware if Applicable
- Patient Protocol/Dose Report

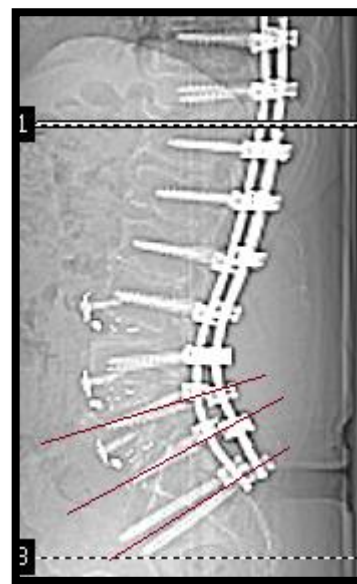

[*Back to Neuro Protocol Page*](#)

CERVICAL SPINE GECK PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	140	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial ST					
Kernel	J30s	J37sMedsmooth	I41s Medium	Cervical	
Window	cerebrum	cerebrum	Spine	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	350/40
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	ASIR	SS10
Window	Cranial bone	Cranial bone	Osteo	Bone	
SAFIRE/ADMIRE	2	0	0	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	1500/450
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	1.25
Reformat				Slice Increment (mm)	1.25
Kernel	J30s	J37sMedsmooth	B30s Med Smooth	Type	Full
Window	cerebrum	Cerebrum	Osteo	ASIR	None
SAFIRE/ADMIRE	2	0	0	Reformat	
Slice Thickness (mm)	1	1	0.75	Algorithm	Detail
Slice Increment (mm)	0.7	0.7	0.5	Window Width/ Level	1500/450
Cor/Sag/Obl				Slice Thickness (mm)	0.625
Kernel	J30s	J37sMedsmooth	I50s Med Sharp	Slice Increment (mm)	0.625
Window	cerebrum	Cerebrum	Osteo	Type	Plus
SAFIRE/ADMIRE	2	0	1	ASIR	None
Slice Thickness (mm)	1	1	1		
Slice Increment (mm)	1	1	1		

THORACIC/LUMBAR SPINE GECK PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660	
Scan Type	spiral	spiral	spiral		Scan Type	spiral	
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20	
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5	
Pitch	0.8	0.3	0.55		Pitch	0.969:1	
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37	
CareDose4D	on	on	on		Scan FOV	Large	
Quality ref mAs	190	125	125		Auto mA range	100-500	
kVp	110				kVp	120	
ref kVp		120	140		Smart mA	off	
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18	
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%	
Axial ST							
Kernel	J30s	J37sMedsmooth	I41s Medium		Axial ST		
Window	cerebrum	cerebrum	Spine		Algorithm	Standard	
SAFIRE/ADMIRE	2	0	0		Window Width/ Level	350/40	
Slice Thickness (mm)	2	2	2		Slice Thickness (mm)	2.5	
Slice Increment (mm)	2	2	2		Slice Increment (mm)	2.5	
Axial Bone					Type	Full	
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp		ASIR	SS10	
Window	Cranial bone	Cranial bone	Osteo				
SAFIRE/ADMIRE	2	0	0		Bone		
Slice Thickness (mm)	2	2	2		Algorithm	Bone Plus	
Slice Increment (mm)	2	2	2		Window Width/ Level	1500/450	
Reformat					Slice Thickness (mm)	2.5	
Kernel	J30s	J37sMedsmooth	B30s Med Smooth		Slice Increment (mm)	2.5	
Window	cerebrum	Cerebrum	Osteo		Type	Full	
SAFIRE/ADMIRE	2	0	0		ASIR	None	
Slice Thickness (mm)	1	1	1				
Slice Increment (mm)	0.7	0.7	0.7		Reformat		
Cor/Sag/Obl					Algorithm	Detail	
Kernel	J30s	J37sMedsmooth	I50s Med Sharp		Window Width/ Level	1500/450	
Window	cerebrum	Cerebrum	Osteo		Slice Thickness (mm)	1.25	
SAFIRE/ADMIRE	2	0	1		Slice Increment (mm)	0.625	
Slice Thickness (mm)	2	2	2		Type	Plus	
Slice Increment (mm)	2	2	2		ASIR	None	

CTDI: ~15-30 mGy

Setup:

- This protocol is dedicated to CT scanning of the Spine, for the region prescribed by the surgeon for each specific case.
- Scout from above area of interest through area of interest

Scan Parameters:

- Scan from above area of interest to below area of interest indicated on referral. Scans need to be completed as one continuous scan. (ex: thoracolumbar case)
- Imaging **must** include contiguous scan through pelvis to the level of the trochanters
- Preferred 200 mm DFOV for CD Data Set (maximum allowed DFOV of 250 mm). Remaining reconstructions preferred DFOV of 12 - 17 cm
- kVp and mAs - according to human size:
 - a. Pediatric: 120kv / 110 mAs
 - b. Adult: 130kv/130mAs
 - c. BMI 35-40: 140kv / 200 mAs

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- Axial Bone
- Axial Soft Tissue
- Coronal
- Sagittal
- Axial Oblique (Lumbar only)
- Right and Left Oblique (Cervical only)
- 1x1 Axial Bone (CD Data Set)
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

CERVICAL SPINE MAZOR PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	140	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set					
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	Axial ST	
Window	Cranial bone	Cranial bone	Osteo	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	350/40
Slice Thickness (mm)	1	1	0.75	Slice Thickness (mm)	1.25
Slice Increment (mm)	0.7	0.7	0.5	Slice Increment (mm)	1.25
Axial ST					
Kernel	J30s	J37s Medsmooth	I41s Medium	Type	Full
Window	cerebrum	cerebrum	Spine	ASIR	SS10
SAFIRE/ADMIRE	2	0	2	Bone	
Slice Thickness (mm)	1	1	1	Algorithm	Bone Plus
Slice Increment (mm)	1	1	1	Window Width/ Level	1500/450
Axial Bone					
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	Slice Thickness (mm)	1.25
Window	Cranial bone	Cranial bone	Osteo	Slice Increment (mm)	1.25
SAFIRE/ADMIRE	2	0	0	Type	Full
Slice Thickness (mm)	1	1	1	ASIR	None
Slice Increment (mm)	1	1	1	Reformat	
Reformat					
Kernel	J30s	J37s Medsmooth	B50s Med Sharp	Algorithm	Detail
Window	cerebrum	Cerebrum	Osteo	Window Width/ Level	1500/450
SAFIRE/ADMIRE	2	0	0	Slice Thickness (mm)	0.625
Slice Thickness (mm)	1	1	0.75	Slice Increment (mm)	0.625
Slice Increment (mm)	0.7	0.7	0.5	Type	Plus
Cor/Sag/Obl					
Kernel	J30s	J37s Medsmooth	I50s Med Sharp	ASIR	None
Window	cerebrum	Cerebrum	Osteo		
SAFIRE/ADMIRE	2	0	1		
Slice Thickness (mm)	1	1	1		
Slice Increment (mm)	1	1	1		

THORACIC/LUMBAR SPINE MAZOR PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	140	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set					
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	Axial ST	
Window	Cranial bone	Cranial bone	Osteo	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	350/40
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
Axial ST				Type	Full
Kernel	J30s	J37s Medsmooth	I41s Medium	ASIR	SS10
Window	cerebrum	cerebrum	Spine		
SAFIRE/ADMIRE	2	0	2	Bone	
Slice Thickness (mm)	2	2	2	Algorithm	Bone Plus
Slice Increment (mm)	2	2	2	Window Width/ Level	1500/450
Axial Bone				Slice Thickness (mm)	2.5
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp	Slice Increment (mm)	2.5
Window	Cranial bone	Cranial bone	Osteo	Type	Full
SAFIRE/ADMIRE	2	0	0	ASIR	None
Slice Thickness (mm)	2	2	2		
Slice Increment (mm)	2	2	2	Reformat	
Reformat				Algorithm	Detail
Kernel	J30s	J37s Medsmooth	B50s Med Sharp	Window Width/ Level	1500/450
Window	cerebrum	Cerebrum	Osteo	Slice Thickness (mm)	1.25
SAFIRE/ADMIRE	2	0	0	Slice Increment (mm)	0.625
Slice Thickness (mm)	1	1	1	Type	Plus
Slice Increment (mm)	0.7	0.7	1	ASIR	None
Cor/Sag/Obl					
Kernel	J30s	J37s Medsmooth	I50s Med Sharp	3D if needed	
Window	cerebrum	Cerebrum	Osteo	Algorithm	Soft
SAFIRE/ADMIRE	2	0	1	Window Width/ Level	400/35
Slice Thickness (mm)	2	2	2	Slice Thickness (mm)	1.25
Slice Increment (mm)	2	2	2	Slice Increment (mm)	0.625

CTDI: ~15-30 mGy

Setup:

- Scout from below the area of interest through the area of interest with the patients arms raised above their head

Scan Parameters:

- Scan from below the area of interest through the area of interest
- Preferred DFOV of 17 cm
- For patients with implanted spinal hardware and/or a BMI \geq 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help to maintain image quality <http://www.nhlbisupport.com/bmi/bminojs.htm>

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay
- See [IV Catheter Guidelines](#)

PACS Series:

- 2x2 Axial Soft Tissue (CD DATA SET)
- 2x2 Axial Bone
- 2X2 Sagittal Spine
- 2x2 Coronal Spine
- Patient Protocol/Dose Report

[*Back to Neuro Protocol Page*](#)

SPINE STEALTH/STRYKER PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660
Scan Type	spiral	spiral	spiral		Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.55		Pitch	0.969:1
Scan FOV	Large	Large	Large		Speed (mm/rot)	39.37
CareDose4D	on	on	on		Scan FOV	Large
Quality ref mAs	190	125	125		Auto mA range	100-500
kVp	110				kVp	120
ref kVp		120	140		Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%
Axial ST						
Kernel	J30s	J37sMedsmooth	I41s Medium		CD Data Set	
Window	cerebrum	cerebrum	Spine		Algorithm	Standard
SAFIRE/ADMIRE	2	0	2		Window Width/ Level	350/40
Slice Thickness (mm)	2	2	2		Slice Thickness (mm)	2.5
Slice Increment (mm)	2	2	2		Slice Increment (mm)	2.5
CD Data Set/Axial Bone					Type	Full
Kernel	J80s verysharp	J70h verysharp	B70s Very Sharp		ASIR	SS10
Window	Cranial bone	Cranial bone	Osteo			
SAFIRE/ADMIRE	2	0	0		Bone	
Slice Thickness (mm)	2	2	2		Algorithm	Bone Plus
Slice Increment (mm)	2	2	2		Window Width/ Level	1500/450
Reformat					Slice Thickness (mm)	2.5
Kernel	J30s	J37sMedsmooth	B70s Very Sharp		Slice Increment (mm)	2.5
Window	cerebrum	Cerebrum	Osteo		Type	Full
SAFIRE/ADMIRE	2	0	0		ASIR	None
Slice Thickness (mm)	1	1	1			
Slice Increment (mm)	0.7	0.7	0.7		Reformat	
Cor/Sag/Obl					Algorithm	Detail
Kernel	J30s	J37sMedsmooth	I50s Med Sharp		Window Width/ Level	1500/450
Window	cerebrum	Cerebrum	Osteo		Slice Thickness (mm)	0.625
SAFIRE/ADMIRE	2	0	1		Slice Increment (mm)	0.625
Slice Thickness (mm)	2	2	2		Type	Plus
Slice Increment (mm)	2	2	2		ASIR	None

CTDI: ~15-30 mGy

Setup:

- Scout from above area of interest through area of interest arms above head

Scan Parameters:

- Scan from above area of interest to below area of interest indicated on referral. Scans need to be completed as one continuous scan. (ex: entire, cervicothoracic, thoracolumbar)
- Preferred 170 mm DFOV
 - *For patients with implanted spinal hardware and/or a BMI \geq 35 it is suggested that increasing kVp, slowing rotation time, and decreasing the pitch will help maintain image quality*

Contrast:

- At the discretion of the Radiologist inject 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 45 second delay

PACS Series Entire Spine:

Cervical ACC#	Thoracic ACC#	Lumbar ACC
*Entire Spine Axial Bone	*Thoracic Axial Bone	*Lumbar Axial Bone
*Cervical Axial Bone	*Thoracic Axial ST	*Lumbar Axial ST
*Cervical Axial ST	*Thoracic Coronal	*Lumbar Coronal
*Entire Spine Coronal	*Thoracic Sagittal	*Lumbar Sagittal
*Entire Spine Sagittal		*Lumbar Axial Oblique
*Cervical Coronal		
*Cervical Sagittal		
*Cervical RT/LT Obliques		

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

PACS Series Cervicothoracic Spine:

3D_Curved Coronal/Sagittal as needed

Cervical ACC#	Thoracic ACC#
*Cervicothoracic Axial Bone	*Thoracic Axial Bone
*Cervical Axial Bone	*Thoracic Axial ST
*Cervical Axial ST	*Thoracic Coronal
*Cervicothoracic Coronal	*Thoracic Sagittal
*Cervicothoracic Sagittal	
*Cervical Coronal	
*Cervical Sagittal	
*Cervical RT/LT Obliques	

PACS Series Thoracolumbar Spine:

Thoracic ACC#	Lumbar ACC#
*Thoracolumbar Axial Bone	*Lumbar Axial Bone
*Thoracic Axial Bone	*Lumbar Axial ST
*Thoracic Axial ST	*Lumbar Coronal
*Thoracolumbar Coronal	*Lumbar Sagittal
*Thoracolumbar Sagittal	*Lumbar Axial Oblique
*Thoracic Coronal	
*Thoracic Sagittal	

****For all spines with hardware-please send Reformat set to Terarecon****


CTDI: ~30-55 mGy

Setup:

- Supine, PA/Lateral scout from below the maxillary sinuses through the frontal sinuses
- BB to be placed behind the Right Ear

Scan parameters:

- Supine helical scan from below the skull base through the entire IAC's
- 15 cm DFOV is preferred
- If the scan is performed with and without contrast, perform routine without contrast and the with contrast only needs 1.0 x 1.0 Bilateral Axial ST/1.0 x 1.0 Bilateral Coronal ST

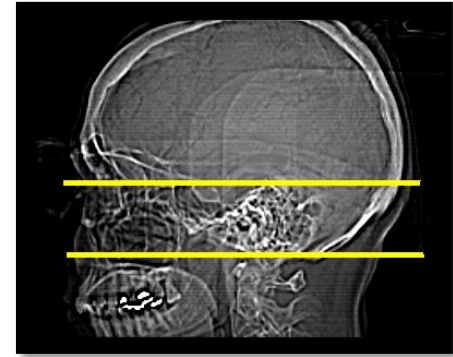

Contrast:

At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 50 second delay


- See [IV Catheter Guidelines](#)

PACS Series:


- Topogram/Scout
- 0.6 x 0.6 Bilateral Axial Bone
- 1.0 x 1.0 Bilateral Axial Soft Tissue
- 0.6 x 0.6 Right Axial Bone
- 0.6 x 0.6 Left Axial Bone
- 0.6 x 0.6 Bilateral Coronal Bone
- 1.0 x 1.0 Coronal Soft Tissue
- 0.6 x 0.6 Right Coronal Bone
- 0.6 x 0.6 Left Coronal Bone
- 0.6 x 0.6 Right Oblique Coronal Bone
- 0.6 x 0.6 Right Oblique Sagittal Bone
- 0.6 x 0.6 Left Oblique Coronal Bone
- 0.6 x 0.6 Left Oblique Sagittal Bone
- Patient Protocol/Dose report

[*Back to Neuro Protocol Page*](#)


Bilateral Bone Axial

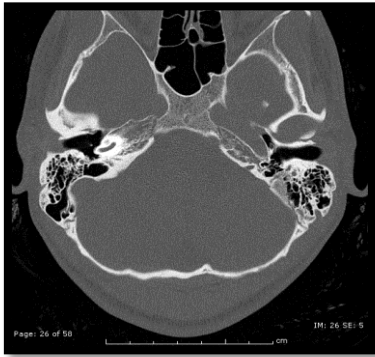


Bilateral Soft Tissue Axial

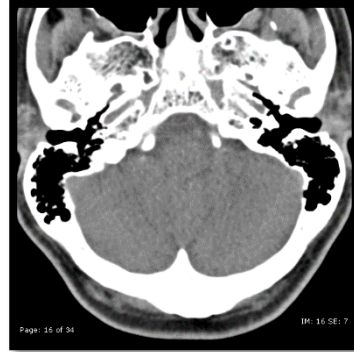


Right Axial Bone

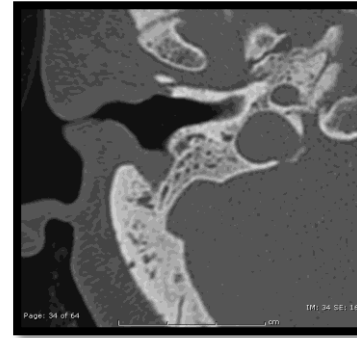


Left Axial Bone

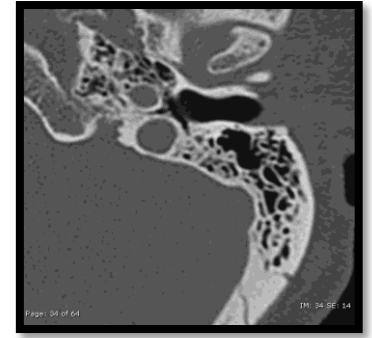

Bilateral Coronal Bone

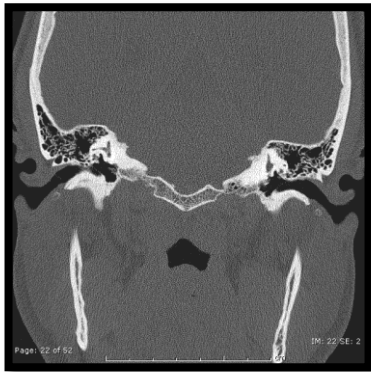


Bilateral Coronal Soft Tissue

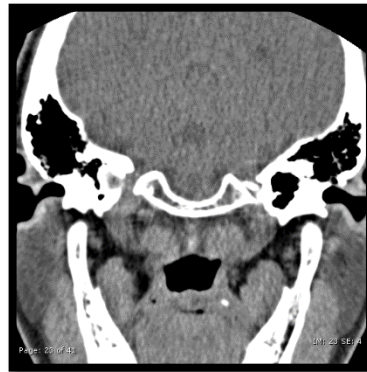

Right Coronal Bone



Left Coronal Bone

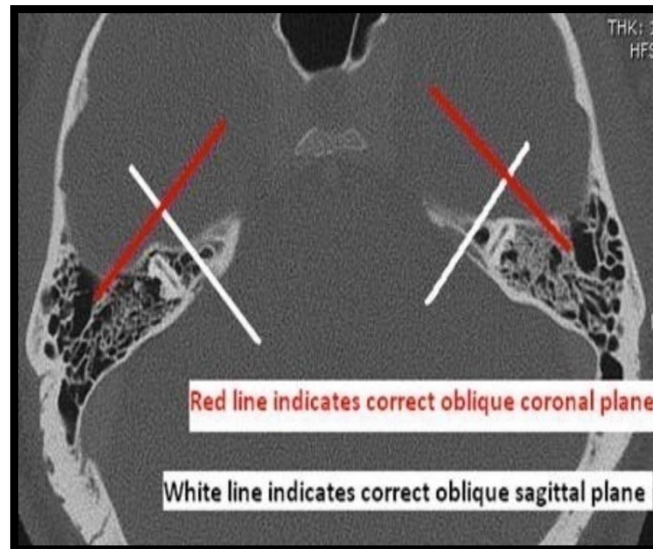

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

TEMPORAL BONE PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	16 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8	Pitch	0.531
Scan FOV	Large	Large	Small	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial ST					
Kernel	J30s	J37s Medsmooth	U30s Medsmooth	Axial Bilateral ST	
Window	cerebrum	cerebrum	Sinuses	Algorithm	Standard
SAFIRE/ADMIRE	2	0	0	Window Width/ Level	400/50
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	1	1	Slice Increment (mm)	1.25
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	V80u Very Sharp	ASIR	SS20
Window	Cranial bone	Cranial bone	Inner Ear	Axial Bilateral Bone	
SAFIRE/ADMIRE	2	0	2	Algorithm	Bone Plus
Slice Thickness (mm)	0.6	0.6	0.6	Window Width/ Level	4000/700
Slice Increment (mm)	0.6	0.6	0.6	Slice Thickness (mm)	0.625
Reformat ST				Slice Increment (mm)	0.625
Kernel	J30s	J37s Medsmooth	U30s Medsmooth	Type	Full
Window	cerebrum	Cerebrum	Sinuses	ASIR	None
SAFIRE/ADMIRE	2	0	0	RT Axial Bone	
Slice Thickness (mm)	0.75	0.75	0.75	Algorithm	Bone Plus
Slice Increment (mm)	0.3	0.3	0.3	Window Width/ Level	4000/700
Reformat Bone				Slice Thickness (mm)	0.625
Kernel	J80s verysharp	J70h verysharp	V80u Very Sharp	Slice Increment (mm)	0.625
Window	Cranial bone	Cranial bone	Inner Ear	Type	Full
SAFIRE/ADMIRE	2	0	2	ASIR	None
Slice Thickness (mm)	0.6	0.6	0.6		
Slice Increment (mm)	0.3	0.3	0.3		

CTDI: ~30-55 mGy

Setup:

- Supine, PA/Lateral scout from below the maxillary sinuses through the frontal sinuses
- BB to be placed on the Right Ear

Scan parameters:

- Supine helical scan from below the skull base through the entire IAC's
- 15 cm DFOV
- If the scan is performed with and without contrast, the bone reconstructions only need to be done on the post-contrast scan


Contrast:

At the discretion of the Radiologist inject 100 ml of 350 mg iodine/ml non-ionic contrast @ 2 ml/sec with a 45 second delay

- See [IV Catheter Guidelines](#)

PACS Series:

- Topogram/Scout
- 0.6 x 0.3 Bilateral Axial Bone (CD Data Set) ****must use 150 DFOV****
- 1.0 x 1.0 Bilateral Axial Soft Tissue
- 0.6 x 0.6 Right Axial Bone
- 0.6 x 0.6 Left Axial Bone
- 0.6 x 0.6 Bilateral Coronal Bone
- 1.0 x 1.0 Coronal Soft Tissue
- 0.6 x 0.6 Right Coronal Bone
- 0.6 x 0.6 Left Coronal Bone
- 0.6 x 0.6 Right Oblique Coronal Bone
- 0.6 x 0.6 Right Oblique Sagittal Bone
- 0.6 x 0.6 Left Oblique Coronal Bone
- 0.6 x 0.6 Left Oblique Sagittal Bone
- Patient Protocol/Dose report

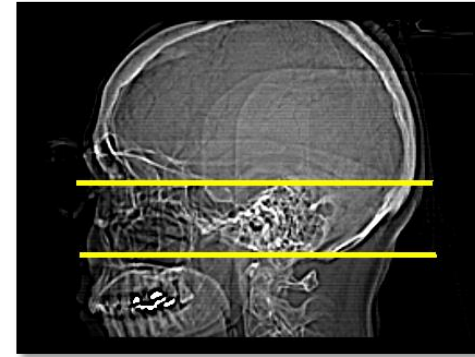

[*Back to Neuro Protocol Page*](#)

TEMPORAL BONE VANDERBILT PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	16 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	0.8	Pitch	0.531
Scan FOV	Large	Large	Small	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set					
Kernel	J80s verysharp	J70h verysharp	V80u Very Sharp	Axial Bilateral ST	
Window	Cranial bone	Cranial bone	Inner Ear	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	400/50
Slice Thickness (mm)	0.6	0.6	0.6	Slice Thickness (mm)	1.25
Slice Increment (mm)	0.3	0.3	0.3	Slice Increment (mm)	1.25
Axial ST				Type	Full
Kernel	J30s	J37sMedsmooth	U30s Med Smooth	ASIR	SS20
Window	cerebrum	cerebrum	Sinuses		
SAFIRE/ADMIRE	2	0	0	Algorithm	Bone Plus
Slice Thickness (mm)	1	1	1	Window Width/ Level	4000/700
Slice Increment (mm)	1	1	1	Slice Thickness (mm)	0.625
Axial Bone				Slice Increment (mm)	0.625
Kernel	J80s verysharp	J70h verysharp	V80u Very Sharp	Type	Full
Window	Cranial bone	Cranial bone	Inner Ear	ASIR	None
SAFIRE/ADMIRE	2	0	2	CD Data Set	
Slice Thickness (mm)	0.6	0.6	0.6	Algorithm	Bone Plus
Slice Increment (mm)	0.6	0.6	0.6	Window Width/ Level	4000/700
Reformat ST				Slice Thickness (mm)	0.625
Kernel	J30s	J37sMedsmooth	U30s Medsmooth	Slice Increment (mm)	0.3
Window	cerebrum	Cerebrum	Sinuses	Type	Full
SAFIRE/ADMIRE	2	0	0	ASIR	None
Slice Thickness (mm)	0.75	0.75	0.75	RT Axial Bone	
Slice Increment (mm)	0.3	0.3	0.3	Algorithm	Bone Plus
Reformat Bone				Window Width/ Level	4000/700
Kernel	J80s verysharp	J70h verysharp	V80u Very Sharp	Slice Thickness (mm)	0.625
Window	Cranial bone	Cranial bone	Inner Ear	Slice Increment (mm)	0.625
SAFIRE/ADMIRE	2	0	2	Type	Full
Slice Thickness (mm)	0.6	0.6	0.6		
Slice Increment (mm)	0.3	0.3	0.3		

CTDI: ~15 - 20 mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Scout and Scan from below the mandible through the orbital roof

DFOV: The axial soft tissue recon is a 25cm DFOV

Contrast:

1. at the discretion of the Radiologist
2. 100 ml of 350 mg/dl non-ionic contrast @ 2 ml/sec with a 60 second delay
3. See [IV Catheter Guidelines](#)

PACS Series:

- Topogram
- 1mm x 1mm Axial Soft Tissue 25 cm DFOV (CD Data set)
- 1mm x 1mm Axial Bone
- 1mm x 1mm Sagittal Bone
- 1mm x 1mm Coronal Bone
- 1mm x 1mm Right Oblique Bone
- 1mm x 1mm Left Oblique Bone
- Patient Protocol/Dose Report

Axial



Sagittal



Coronal



RT Oblique



LT Oblique



[*Back to Neuro Protocol Page*](#)

TMJ PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64		Scanner	Optima 660	
Scan Type	spiral	spiral	spiral		Scan Type	spiral	
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6		Detector Coverage (mm)	20	
Rotation Time (sec)	0.6	0.5	1		Rotation Time (sec)	0.5	
Pitch	0.8	0.3	0.55		Pitch	0.531	
Scan FOV	Large	Large	Small		Speed (mm/rot)	39.37	
CareDose4D	on	on	on		Scan FOV	Large	
Quality ref mAs	190	125	125		Auto mA range	100-500	
kVp	110				kVp	120	
ref kVp		120	120		Smart mA	off	
Optimize Slider position		3 w/o contrast	3 w/o contrast		Noise Index	18	
Optimize Slider position		7 w/ contrast	7 w/ contrast		ASIR	20%	
Axial ST							
Kernel	J30s	J37sMedsmooth	J30s Med Smooth		Axial Bilateral ST		
Window	cerebrum	cerebrum	Sinuses		Algorithm	Standard	
SAFIRE/ADMIRE	2	0	2		Window Width/ Level	380/40	
Slice Thickness (mm)	1	1	1		Slice Thickness (mm)	1.25	
Slice Increment (mm)	1	1	1		Slice Increment (mm)	1.25	
Axial Bone					Type	Full	
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp		ASIR	SS20	
Window	Cranial Bone	Cranial Bone	Cranial Bone				
SAFIRE/ADMIRE	2	0	1		Axial Bilateral Bone		
Slice Thickness (mm)	1	1	1		Algorithm	Bone Plus	
Slice Increment (mm)	1	1	1		Window Width/ Level	1500/450	
Cor/Sag/Obl					Slice Thickness (mm)	1.25	
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp		Slice Increment (mm)	1.25	
Window	Cranial Bone	Cranial Bone	Cranial Bone		Type	Full	
SAFIRE/ADMIRE	2	0	1		ASIR	None	
Slice Thickness (mm)	1	1	1				
Slice Increment (mm)	1	1	1		CD Data Set if needed		
					Algorithm	Standard	
					Window Width/ Level	380/40	
					Slice Thickness (mm)	0.625	
					Slice Increment (mm)	0.625	
					Type	Full	
					ASIR	SS20	

CTDI: ~15 - 20 mGy

Place skin marker on the patient's right cheek prior to scanning

Setup:

- Scout and Scan from below the mandible through the orbital roof

DFOV: The axial soft tissue recon is a 20cm DFOV (may be adjusted to best fit patient anatomy)

Pre Scan Checklist:

- See Attached

Procedure:

- See Attached

PACS Series:

- Topogram
- 0.6 mm x 0.6 mm Axial Soft Tissue 20 cm DFOV (CD Data set)
- 1mm x 1mm Axial Bone
- 1mm x 1mm Sagittal Bone/ST
- 1mm x 1mm Coronal Bone/ST
- Patient Protocol/Dose Report



TMJ CONCEPTS

6059 King Drive, Ventura, CA 93003, USA
Phone (805) 650-3391 or Toll Free (800) 504-9527

TMJ Concepts CT Scanning Protocol

This protocol is to ensure that accurate 3-D bone models can be created and used for the design and manufacture of patient-fitted temporomandibular joint prostheses. It does not define the use of or parameters for cone beam scanners. Consult with TMJ Concepts regarding cone beam scanning parameters.

Please review the following information before proceeding with the scanning process. If you have any questions, contact TMJ Concepts at 805-650-3391 (Toll free 800-504-9527) prior to scanning the patient. TMJ Concepts can be visited on the web at www.tmjconcepts.com.


Pre-Scan Checklist

- Remove any jewelry that is in the scan area.
- Stabilize the patient with sponges, tape, and any other accessories that will not cause injury to the patient or affect the quality of the scan. It is extremely important that the patient does not move or swallow during the scanning process.
- Position the patient so that he/she lay supine.
- Patient should be scanned in good occlusion when possible. Patients that cannot achieve a good occlusal position should be scanned with a bite jig or other apparatus to stabilize and separate the teeth. If there is any question regarding what is appropriate, please contact the ordering surgeon.

Procedure

- Inform the patient when the actual scanning process starts. Instruct them to not move or swallow until the scan is complete. If there is movement, the patient must be re-scanned.
- Take a scout view and locate the first slice position. Make sure the head is positioned symmetrically so that the first slice is positioned correctly for both the left and right TMJ.
- Start the scan so that it includes both the sella and nasion. Be sure that both inferior orbital borders and EAC's are included. Scan through the tip of the chin.
- Scans must **not** be provided with greater than 1mm slice intervals. If your standard scanning parameters are .5mm, .625mm, or .75mm slice intervals, please provide the greatest level of detail scanned. Do **not** reformat axial slice data into a different slice interval.
- Only axial image data is required. If possible, retain the raw CT data until the scan has been reviewed by TMJ Concepts.
- Data should be archived onto a CD in an uncompressed DICOM format using a standard-type algorithm. Do **not** use a Detail or Bone algorithm. Preferred algorithms for common scanners are shown in the table at the right.
- Label the disk with surgeon name, patient name, date of scan, technician name, scanner type, scan site name and phone number.
- Send data to TMJ Concepts via overnight shipping or via ftp or other data transfer utility. For help with data transfer, please contact TMJ Concepts.

Helical Scanning Parameters	
Scan Area	TMJ/Mandible/Maxilla (per diagram below)
Algorithm	Standard (Do not use Detail or Bone)
	Preferred Algorithms GEStandard PhillipsB SiemensH30s ToshibaFC30 or FC03*
FOV	20 cm (may be adjusted to best fit patient anatomy)
Pitch	1:1
Slice Interval	0.5mm to 1mm Do Not Reformat
Slice Thickness	Same as slice interval
Contrast	Scan without contrast
Gantry Tilt Angle	0
Archival	Uncompressed DICOM image data on CD

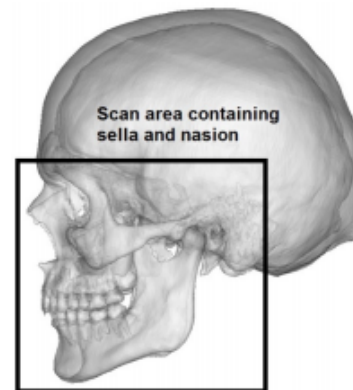

TMJ CONCEPTS PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	0.6	0.5	1	Rotation Time (sec)	0.5
Pitch	0.8	0.3	1	Pitch	0.969:1
Scan FOV	Large	Large	Small	Speed (mm/rot)	39.37
CareDose4D	on	on	on	Scan FOV	Large
Quality ref mAs	190	125	125	Auto mA range	100-500
kVp	110			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3 w/o contrast	3 w/o contrast	Noise Index	18
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
CD Data Set					
Kernel	J30s	J37sMedsmooth	J30s Med Smooth	Axial ST	
Window	Cerebrum	Cerebrum	Sinuses	Algorithm	Standard
SAFIRE/ADMIRE	2	0	2	Window Width/ Level	380/40
Slice Thickness (mm)	1	3	0.6	Slice Thickness (mm)	1.25
Slice Increment (mm)	1	3	0.6	Slice Increment (mm)	1.25
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp	ASIR	SS20
Window	Cranial Bone	Cranial Bone	Cranial Bone		
SAFIRE/ADMIRE	2	0	1	Axial Bone	
Slice Thickness (mm)	1	3	1	Algorithm	Standard
Slice Increment (mm)	1	3	1	Window Width/ Level	700/80
Cor/Sag ST				Slice Thickness (mm)	0.75
Kernel	J30s	J37sMedsmooth	J30s Med Smooth	Slice Increment (mm)	0.5
Window	Cerebrum	Cerebrum	Sinuses	Type	Full
SAFIRE/ADMIRE	2		0	ASIR	SS20
Slice Thickness (mm)	3	3	1		
Slice Increment (mm)	3	3	1	CD Data Set/ST Reformat	
Cor/Sag Bone				Algorithm	Standard
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp	Window Width/ Level	380/40
Window	Cranial Bone	Cranial Bone	Cranial Bone	Slice Thickness (mm)	0.625
SAFIRE/ADMIRE	2	0	1	Slice Increment (mm)	0.625
Slice Thickness (mm)	1	3	1	Type	Plus
Slice Increment (mm)	1	3	1	ASIR	SS20

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*

CTDI: ~ 35-60 mGy

Setup

- Head First Supine
- Keep slices as orthogonal to the leads as possible



Exam:

- Routine Brain without contrast
- Start scans at the bottom of the skull base and scan through the top of the head
- Do not cut off lead tip(s)

DFOV: Preferred 20 cm (Range 18-22)

PACS Series:

- 1x1 Brain
- 1x1 Bone (Only needed on one series not both)
- 1x1 Coronal ST
- Patient Protocol/Dose Report

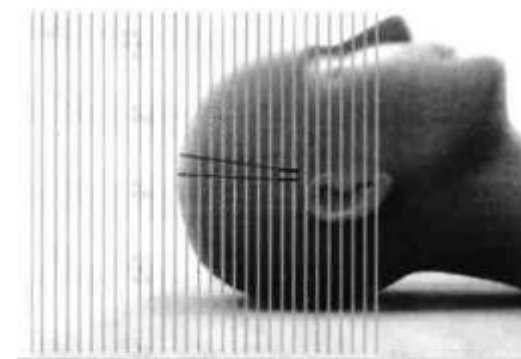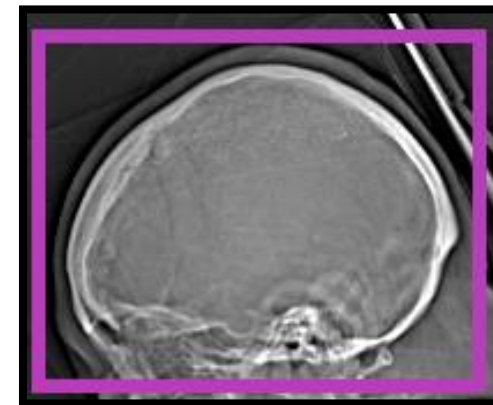

[*Back to Neuro Protocol Page*](#)

HEAD DBS LEAD PROTOCOL

Scanner	Perspective	Definition AS 40	Definition AS 64	Scanner	Optima 660
Scan Type	spiral	spiral	spiral	Scan Type	spiral
Detector Configuration	32 x 0.6	64 x 0.6	64 x 0.6	Detector Coverage (mm)	20
Rotation Time (sec)	1.5	1	1	Rotation Time (sec)	0.5
Pitch	0.55	1	0.55	Pitch	0.969:1
Scan FOV	Large	Large	Large	Speed (mm/rot)	39.37
CareDose4D	off	off	off	Scan FOV	Large
Quality ref mAs	190	225	275	Auto mA range	100-500
kVp	130			kVp	120
ref kVp		120	120	Smart mA	off
Optimize Slider position		3w/o contrast	3 w/o contrast	Noise Index	10
Optimize Slider position		7 w/ contrast	7 w/ contrast	ASIR	20%
Axial Brain					
Kernel	J37sMedsmooth	J37sMedsmooth	J37s Med Smooth	Recon 1 Brain	
Window	cerebrum	cerebrum	cerebrum	Algorithm	Standard
SAFIRE/ADMIRE	0	0	2	Window Width/ Level	80/35
Slice Thickness (mm)	1	1	1	Slice Thickness (mm)	2.5
Slice Increment (mm)	1	1	1	Slice Increment (mm)	2.5
Axial Bone				Type	Full
Kernel	J80s verysharp	J70h verysharp	J70h Very Sharp	ASIR	SS30
Window	Cranial bone	Cranial bone	Cranial bone		
SAFIRE/ADMIRE	0	0	1	Recon 2 Bone	
Slice Thickness (mm)	1	1	1	Algorithm	Bone
Slice Increment (mm)	1	1	1	Window Width/ Level	3000/800
Coronal ST				Slice Thickness (mm)	2.5
Kernel	J37sMedsmooth	J37sMedsmooth	J37s Med Smooth	Slice Increment (mm)	2.5
Window	Cerebrum	Cerebrum	Cerebrum	Type	Full
SAFIRE/ADMIRE	0	0	2	ASIR	SS20
Slice Thickness (mm)	1	1	1		
Slice Increment (mm)	1	1	1	Recon 2 Trauma Reformat	
				Algorithm	STND
				Window Width/ Level	100/50
				Slice Thickness (mm)	1.25
				Slice Increment (mm)	0.625
				Type	Full
				ASIR	None

Protocol Review

CT Protocols are reviewed by the Radiation Safety Protocol Committee.

Committee members consists of ARA Radiation Safety Officer, Radiologists, ARA Outpatient Imaging Center Directors, Manager of Quality, Safety and Risk Management and Lead CT Technologists

Protocol(s) Review Date
09/04/2024

**Protocol designed to minimize the amount of radiation while maximizing the yield and produce diagnostically acceptable image quality*